





ULTRASONIC TRANSIT TIME FLOWMETER

TTFM100W SERIES

STATIONARY TYPE




INSTRUCTION MANUAL

Ultrasonic Transit Time Flow meter TTFM100 Series

1	WO	RKING PRINCIPLE	6
	1.1	TYPICAL USE	7
	1.2	PACKING LIST	
	1.2.1	Connections	
2	INST	TALLATION AND OPERATION	12
	2.1	MEASURING POINT	12
	2.2	REQUIRED INFORMATION	
	2.3	A PRACTICAL EXAMPLE OF RAPID SETTINGS	13
	2.3.1	T T	
	2.3.2		
	2.4 2.5	INSTRUCTIONS FOR CLAMP-ON SENSORS MOUNTINGTRANSDUCER MOUNTING METHODS	
	2.5 2.5.1		
	2.5.2		
	2.5.3	O Company of the comp	
	2.5.4		
	2.5.5	1 0 , 33	
	2.5.6	Relation between calculated and measured transit time	
3	DISI	PLAY WINDOWS	35
	3.1	FLOW RATE- TOTALIZERS MENU	35
	3.2	INITIAL SETTING MENU	
	3.3	FLOWRATE UNITS MENU	
	3.4	OPTIONAL SETTING MENU	
	3.5	INPUTS/ OUTPUTS MENU	
	3.6 3.7	DIAGNOSTICS MENUOTHER DISPLAY MENU	
	3.8	FLOW RATE - TOTALIZERS MENU ANALYSIS	
	3.9	INITIAL SETTING MENU ANALYSIS	
	3.10	FLOWRATE UNITS MENU ANALYSIS	
	3.10.		
	3.11	DIAGNOSTICS MENU ANALYSIS	
	3.12	OTHER DISPLAYS MENU ANALYSIS	68
4	DIAGNOSTICS AND PROBLEM SOLVING		
	4.1	AUTOTEST DURING SWITCHING ON AND POSSIBLE SOLUTIONS	70
	4.2	ERROR CODES, CAUSES AND SOLUTIONS DURING FUNCTIONING	71
5	COM	MUNICATION WITH A PC AND/ OR DATA LOGGING	72
	5.1	DIRECT CONTROLS – PROTOCOL	72
6	APP	ENDIX	74
-	6.1	SOUND SPEEDS IN SOLIDS	
	6.2	SOUND SPEEDS IN FLUIDS	
	6.3	SOUND SPEEDS IN WATER AT SELECTED TEMPERATURES	
	6.4	PIPE SIZE DATA	92
7	EC-	DECLARATION OF CONFORMITY	97
U	LTRASC	ONIC TRANSIT TIME FLOW METER	100
		SERIES	
		LOGGER	
	-	RED HARDWARE	
2.	INITIA	L SETTINGS FOR DATA LOGGER FUNCTION	101

Ultrasonic Transit Time Flow meter TTFM100 Series

2.1 TTFM100 – TTFM100B SETTINGS (WALL MOUNT AND PORTABLE)	102
2.2 HARDWARE CONNECTIONS BETWEEN TTFM100 & PC	
2.3 CONNECTION SOFTWARE BETWEEN THE PC & THE TTFM100 SERIES	
2.4 Data logging in .txt - TEXT FORMAT	
3. HOW TO USE EXCEL $^{\odot}$ TO READ THE .TXT DATA	110
3.1 How to import .TXT files in Excel [©]	111
3 2 AN EVAMPLE OF FLOW PATE RAD CRADH	

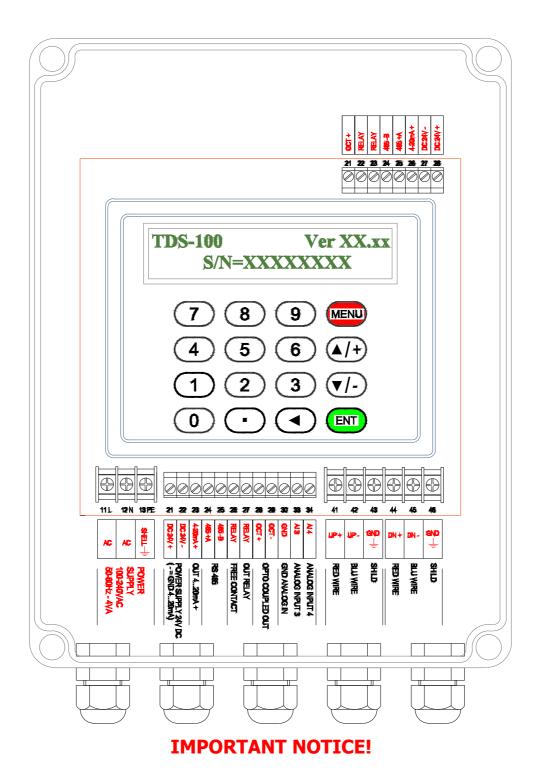

EACH DEVICE HAS TO BE CONNECTED TO THE SENSORS WITH THE SAME SERIAL NUMBER OF THE DEVICE.

THE SERIAL NUMBER IS WRITTEN ON THE ID LABEL OF THE DEVICE

THE SERIAL NUMBER IS WRITTEN ON THE ID LABEL OF THE DEVICE AND SENSORS.


INTRODUCTION

Thanks for buying an Ultrasonic Transit Time Flow meter TTFM100-NG series.

The device measures flow rate by calculating the spreading time of an ultrasonic wave in a liquid, going upstream and downstream into a pipe. This flow meter is mostly used to measure the flow rate of homogeneous fluids, with a very little percentage of suspended solids and possibly without gas bubbles.

Its peculiar installation makes these devices suitable for measuring aggressive fluids (acids, basic and dissolvent) or very soiling fluids (oil and fuels).

The measuring system is composed of a couple of ultrasonic transducers acoustically coupled to the external pipe's wall (it is also possible to use transducers in direct contact with fluid to be measured) and a HOST unit elaborating the sent and received signals from the transducers. The HOST unit has a DSP microprocessor; it gives signals to interfacing with the process or the control systems.

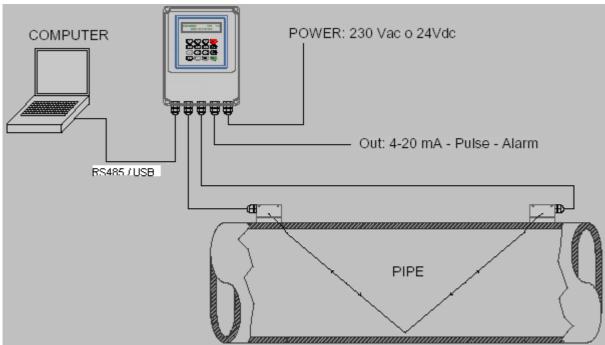

The devices main features are:


- Clamp-on sensors: it is not necessary to stop the flow to install them. Or Insertion sensors.
- AC and DC supply: 230 VAC and 24 VDC.
- The time difference during the measuring process could be 0.2 ns.
- Analog (4-20 ma), pulses (relays), frequency (OCT) and RS232 outputs.
- All the measures could be driven to the RS485 in order to save data into a PC or a serial printer.

1 WORKING PRINCIPLE

When the ultrasonic wave spreads in a liquid, the flow will cause a changing in the spreading time depending on downstream or upstream current.

The ultrasonic wave going towards the same directions of the flow increases the spreading speed, while the ultrasonic wave going towards the opposite side of the flow decreases the spreading speed.

If the difference between the two spreading times is accurately measured, it would be possible to calculate the flow speed (see the following picture).

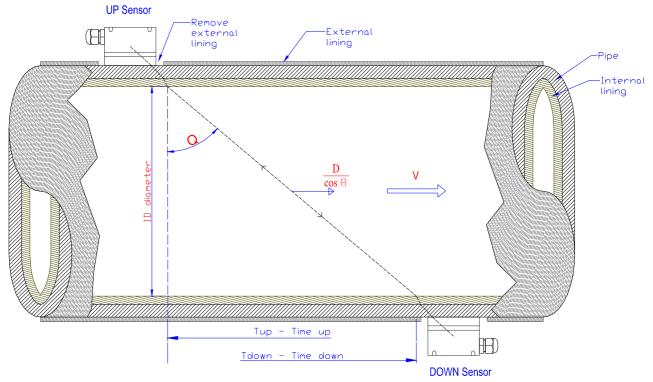

The measures are taken by 2 sensors in direct contact with the pipe's external surface.

One sensor is placed on the upper side of the pipe's external surface, one sensor is placed on the lower side of the pipe's external surface.


The sensors positions could look like a "Z" or like a "V" or a "W", if the pipe has a small diameter (in the previous sketch, the sensors are "Z" mounted).

The sensors are alternatively used to receive the ultrasonic pulses sent through the way pipe - fluid - pipe.

The difference between the transmitted and received signals upstream and downstream is calculated as follows:

(1) (2) (3)
$$Tup = \frac{\frac{M*D}{COS\Theta}}{\frac{COS\Theta}{Co + VSIN\Theta}} \qquad Tdown = \frac{\frac{M*D}{COS\Theta}}{\frac{COS\Theta}{Co - VSIN\Theta}} \qquad V = \frac{M*D}{SIN2\Theta} * \frac{\Delta T}{Tup*Tdown}$$

Typical timing signal



T₁ Downstream time

T₂ Upstream time

 $DT = T_2 - T_1$

Where:

M Spreading time

D Pipe's internal diameterΘ Transmission angle

Co Sound spread speed through the fluid in static conditions

Tup Positive spreading time Tdown Negative spreading time

V Flow Velocity

The DT value is the difference of the spreading time into a homogenous fluid without gas bubbles.

The equation (3) for calculating the average speed "V" could be used for all the types of fluids in ideal conditions. The fluid speed measuring is in fact conditioned by different factors which make the precision decrease: for example the dumps on the pipe are internal walls: they change the measuring principle of the transit time flow meter.

TTFM100 series has are a lot of solutions trying to solve these problems, compensating the temperature influence, the dumped internal walls and the asymmetry in the speed distribution, in order to measure in critical conditions too.

It is possible to adjust the zero point of the device: if the fluid is in static conditions, this operation makes the repeatability precision increase until reaching values near to 0.5%.

1.1 TYPICAL USE

- Water treatment, slurry and process water pumping;
- Oil and chemical industries;
- Hydro-electric, cooling, anti-fire stations;
- Extraction industries;
- Food, paper and pharmaceutical industries;
- Car industries:
- Flow balancing;

• Heat measuring in central systems.

1.2 PACKING LIST

 Ultrasonic Transit Time Flow meter (fixed or portable) 	1pcs
• Standard Clamp-on sensors TS2	2pcs
• Standard Clamp-on sensors TM1	2pcs
• Standard Clamp-on sensors TL1	2pcs
Acoustic coupling	1pcs
Sensors mounting kit (optional)	1pcs
Quality certification	1pcs
Instruction Manual	1pcs


* DEPENDING FROM THE TYPE OF SENSORS ORDERED BY THE CUSTOMER.

1.1 TECHNICAL FEATURES

ITEM		PERFORMANCE
	Material	Steel, Stainless Steel, cast iron, plastic, with smooth walls, with rough walls, with very thin walls.
PIPE	Internal Diameter	20 ~ 6000 mm.
	Pipe length	Upstream: bigger than 10D and 50D far from the pump, downstream: bigger than 5D.
	Туре	Potable water, sea water, other liquids with few suspended solids.
FLUID	Turbidity	Smaller than 10000ppm (mg/l) with a few air bubbles.
	Temperature	-20°C ~ +80°C, without ice at low temperatures.
SPEED	Speed	-16 m/s ~ +16 m/s
SENSORS	Туре	 Standard – TS2 DN15DN300 mm Standard – TM1 DN50DN1000 mm Standard – TL1 DN300DN6000 mm Insertion type B > 50 mm < 2000 mm for under charge applications. Min. temp.
		-40°C, max temp. 160°C, max pressure 60 bars.
		4. Sensors pre-mounted between flanges F type from DN50 to DN1000, PN16 until

DN400, PN10 until DN1000, min. temp.			
		40°C, max. Temp. 160°C.	
	Cable lengths	Min. 5 m, max. 500 m.	
SENSORS	Mounting methods	"V" Method: for pipes with small diameter, until DN400 mm. "Z" Method: for pipes with big diameters, bigger than DN250. "W" or "N" Method: suitable for very small pipes, DN15100.	
	Display	Alphanumeric 2 x 20 digits LCD back lighted.	
	Keypad	4 x 4	
	Mounting	Wall mounting.	
	Input	5 current loop 4 - 20 mA, 0.1% accuracy.	
FLOWMETER	Outputs	Selection 4 - 20 mA or 0 - 20 mA current loop, 0.1% accuracy.	
TEOWNETEN		Serial port RS485.	
		Programmable output frequency: 129999 Hz.	
		Output relays 1A/125VAC or 2A/30VDC for volume pulses or alarms.	
	Dimensions	Fixed type: 251 x 92 x 80 mm.	
	Weight	Fixed type: 3.1 kg	
ENVIRONMENTAL	Temperature	Device: -20°C+40°C	
AND		Sensors: -20°C+80°C	
OPERATIONG	Humidity	Device: 85% RH (40°C)	
CONDITIONS		Sensors: 98% RH (40°C), possible functioning in water less deep than 2 m.	
		+/- 1% (after calibration)	
MEASURING	ACCURACY	Repeatability: +/-0.2%0.5% at 0.616mt/s	
		Linearity: 0.5%	
		NA: 1 FOO :11: 1	
		Min measuring cycle: 500 milliseconds	
		Min measuring cycle: 500 milliseconds 100 - 240 VAC 50/60Hz – 4 VA or	
POWER 9	SUPPLY		
POWER S	SUPPLY	100 - 240 VAC 50/60Hz – 4 VA or	

1.2 WIRING AND CONNECTIONS

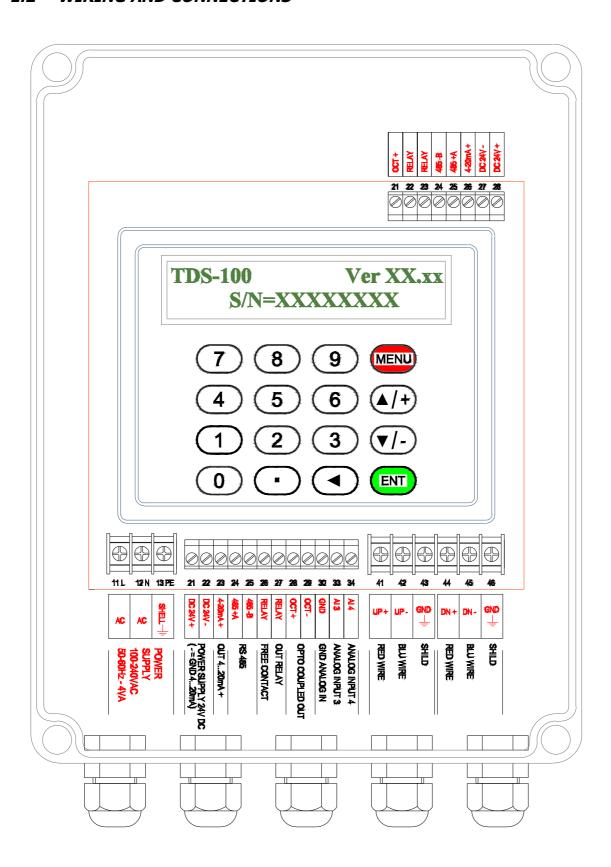

Please use the connector, from left to right, in the following way:

- Clamps "AC IN L", connection for AC supply, phase/live.
- Clamps "AC IN N", connection for AC supply, neutral.
- Clamps "AC IN PE", earth connection/chassis-shell common.
- Clamps "DC IN" respectively + and for 24 VDC supply.
- RS485- COM PORT communication port.
- Clamps "RELAY" extractable, vertical type, suitable for the connection of the pulse output or alarm.
- Clamps "OCT" suitable for the connection of the frequency output, pulse output, o for the alarm.
- Clamps "AI1, AI2, GND" suitable for the connection of the temperature transmitters in LOOP in 4-20 mA.
- Clamps for ultrasonic sensors respectively up sensor and down sensor. Connect
 the red wire to the positive pole, and the black wire to the negative pole, the
 display should be connected only to the GND clamp. Repeat the same connection
 for both sensors.
- Clamps "4 20 mA" connect the signal for a graphic recorder or a process control with 4-20 ma input.

1.2.1 Connections

The kind of connection the number of connections, both depend from the application the flow meter is used for.

The minimum necessary connections are:

- Electrical supply AC or DC
- Ultrasonic UP and Down sensors

Warning!!!!!

The sensors must be connected to their clamps only after having momentarily short circuit the red and black cables in order to discharge electrostatic charges generated during the sensors movement.

The crystal inside the transducer acts as a converter and makes the mechanical energy become electrical energy during the mounting.

When the sensors are connecting to the clamp-house, the electrostatic charges into the capacitor, could damage seriously the measuring circuit of the device.

- 4-20 ma output and/or frequency and/or pulses signals
- Temperature measure for calorimeter
- RS485 connection for data saving.

2 INSTALLATION AND OPERATION

The ultrasonic flow meter mounting is a quite simple method. It is only necessary to determine the mounting point in the pipe and knowing some information about the pipe's dimension.

2.1 MEASURING POINT

It is very important to select the right measuring point. The fluid has to be a measurable fluid and the pipe should be indicated among the foreseen for this technology. Please do not hesitate to contact B.M. TECNOLOGIE INDUSTRIALI for any further clarification.


Please proceed as follows:

- 1) Select the measuring point on the pipe, in order to have a fluid free from turbulences.
- 2) The distance of measurement point upstream is 10D, downstream is within 5D. If there is valve upstream, it is suggested to increase the distance up to 30 D.
- 3) Actually, the device could be installed into pipes with lining, but it is suggested to avoid it above all if the pipe is old or damaged.
- 4) Select suitable pipes with a uniform kit in order to improve measure and precision.

2.2 REQUIRED INFORMATION

- 1) Pipe's external diameter.
- 2) Pipe's internal diameter.
- 3) Pipe's material or speed of sound through this material.
- 4) Internal lining (If present).
- 5) Fluid type (or speed of sound through this fluid).
- 6) Transducer type.
- 7) Transducer mounting method (V, Z method or W for little pipe).

Now, in M25 menu it will be possible to see the right mounting distance between the transducers.

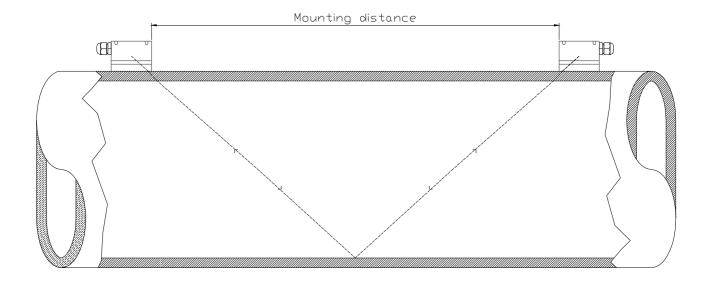

2.3 A PRACTICAL EXAMPLE OF RAPID SETTINGS

The following example represents an application into a DN 400 carbon steel pipe, without lining, with "V" mounted sensors.

IMPORTANT NOTICE: WHEN THE SET-UP IS FINISHED, THE USER <u>MUST</u> RETURN TO MENU 26 AND SELECT OPTION <u>1. SOLIDIFY SETTINGS</u>, AND THEN PRESS ENTER. IN THIS WAY THE PARAMETE WILL BE SAVED EVEN IF THE POWER SUPPLY GOES OFF.

2.3.1 Fluid & pipe's features

This is a zinc pipe, so its thickness is not a problem. It is also important to measure the perimeter of the pipe: it should be 1286 mm. The pipe is PN10 and it will measure potable water.

2.3.2 Data entry

Switch on the device and it will display the following:

Then it will display, (it depend by the last switch off) for example:

0.0000 m 3/h * IFlow No Signal Detected The transducers are not mounted yet and their mounting distance will be displayed only after the programming. Actually the device detects no signals. Press and the device will display: Flow 0.0000 m3/h * IWindow No. Press and the device will display the content of window no. 10. Pipe Outer Perimeter XXXX mm **Press** and that display will turn into this display: Pipe Outer Perimeter 1286 mm If you press a wrong digit, press and the device will display: Pipe Outer Diameter XXX.XXX mm and the device will display: Pipe Wall Thickness X.X mm+ ENT 5 and the it will display: Pipe Wall Thickness 6.5 mm

and the device will display:

Pipe Inner Diameter 396.347 mm

The device calculated the displayed value basing on the settings made.

If you want, it is possible to press parameters calculated until now.

Press and the device will display:

Pipe Material [14]
1. Stainless Steel

The displayed material depends from the material of the pipe you are using.

Press and "1" and will be blinking.

Pipe Material [14]

Stainless Steel

Select the material by using the digits

Pipe Material [14 >0. Carbon Steel

Press ENT and and the device will display:

Liner Material [16]
0. None, No Liner

In this case, the pipe has no internal lining, so the value $\ensuremath{\text{``0''}}$ is correct.

Press and the device will display:


Fluid Type [20 0. Water (General)


Press and the device will display:

Transducer Type [23]
10. Standard-M1


NOTE:

The standard supplied sensors are M sensors, permitting measures in pipes from DN50 up to DN1000. It is possible to ask for different kind of sensors, depending on the measures to be done.





Press and the device will display:




The displayed value corresponds to the sensors distance, as shown in par. 2.2. Now it is possible to mount the transducers, as shown in the following par. 2.4.

Press and the device will display:



Press and the device will display:



Press to go through the parameters:

Save / Load parameters

To Browse

Or set up one of the 9 (0...8) preset configurations:



Press and the device will display:

Save / Load parameters

Entry to SAVE

Press and the device will display:

Save / Load parameters
0: 409,347 mm, Carbon

This setting refers to the just set configuration: DN400 carbon steel pipe.

Press and the device will display:

Save / Load parameters
Entry to SAVE

Press MENU, 1, ENT and the device will display:

Flow 0.0000 m3/h *I No Signal Detected

Now it is possible to mount the transducers.

2.4 INSTRUCTIONS FOR CLAMP-ON SENSORS MOUNTING

If you ordered Clamp-on sensors type TTS100-S1-NG, TTS100-M1-NG, TTS100-L1-NG, TTS100-S1-NG-HT, TTS100-M1-NG-HT it is very important to follow the instructions listed below in order to install the sensors correctly:

1. In order to install the sensors, check if the pipe has features which could affect the measure, i.e. rust, dirt...



2. if so, please use a marker



To trace an area bigger than the sensors area



This will help you to delimit the area to be cleaned.

3. pls clean it by using one of the following tools:



Or



Or



4. the pipe portion in which the sensor will be mounted should be completely clean:



Now the pipe is ready and the clamp-on sensors could be installed.





Or, if it is not possible to measure the diameter, please measure the **pipe's circumference**:



6. Measure the pipe's thickness.
This could be done by using our **Thickness Gauge TT100-TM8812-NG**



Before using the Thickness Gauge sensors, please remember to use the coupling grease:



Otherwise, the sensors could loose grip to the pipe.



Now place the Thickness Gauge TT100-TM8812-NG sensor and measure the pipe's thickness:



- 7. when the following values have been entered into device's menus:
 - pipe's diameter (MENU 11) or pipe's circumference (MENU 10)
 - pipe's thickness (MENU 12)
 - type of clamp-on sensors to be used (MENU 23)
 - type of sensors mounting method (MENU 24)

The device will display the distance at which the sensors should be mounted (MENU 25).

8. Now it is possible to start the sensors installation. Please remember to use the coupling grease:



Otherwise, the sensor could loose grip to the pipe.




9. now sensors could be installed by using a fixing bracket:



10. it is necessary to install the sensors according to the distance value the device displays in MENU 25:



11. now the clamp-on sensors installation is complete:

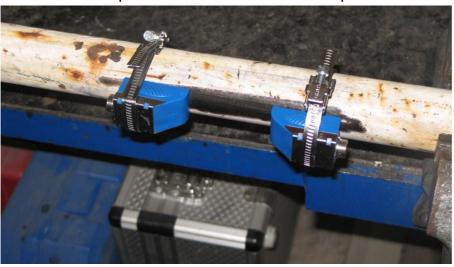

2.5 TRANSDUCER MOUNTING METHODS

The transducers mounting positions are related to the pipes diameters and to the type of sensors we have, so V and Z methods are the most common. By the way, V mounting is suggested.


This type of flow meter enables the N and W mounting methods too.

The letters stands for the number of signal crossings from one transducer to another.


- Z= one crossing. Suitable for pipes > DN250 mm or even smaller.
- V= two crossings. It is the easiest mounting method for pipes until DN600-800 mm with TL-1 or TM-1 transducers.
- N= three crossings. Suitable for small pipes, DN100 or less, with TL-1 transducers.
- W= four crossings. Suitable for DN20 pipes with TS-2 and TL-1 transducers.

The follow sketch shows the various mounting solution for the transducers.


"Z" mounting

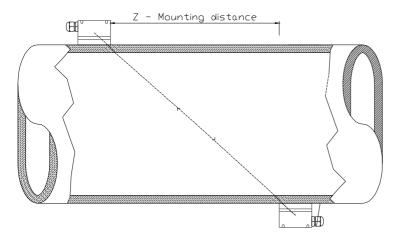


"V" mounting

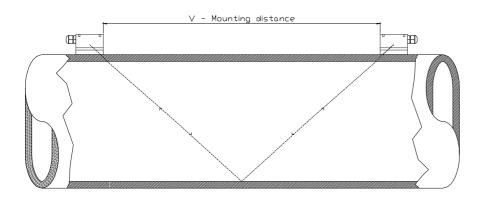

"N" mounting

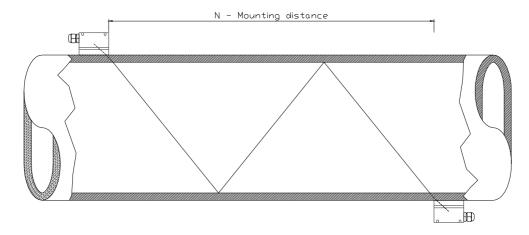

"W" mounting

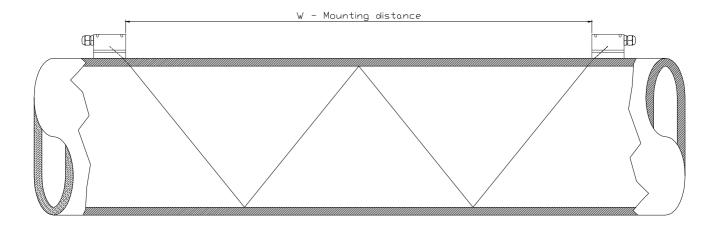


It is possible to apply to almost all the cases the V mounting method: it is the most simple and rapid one.


It is suggested to select the Z mounting method only if the signal strength, UP and DN is smaller than 60 and Q value is smaller than 60, see MENU "90".

In this case $\ \ Z''$ mounting is suggested.

2.5.1 "V" mounting

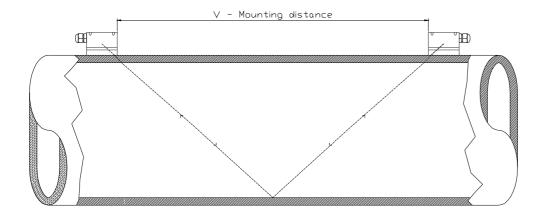

The "v" method uses a bounce into the pipe and the ultrasonic wave goes through more distance. The measuring principle is based on the difference of time and through a "V" distance, the time needed is bigger and the precision higher. In case of horizontal mounting, it is suggested to avoid mounting the sensors on the top or on the bottom of the pipe. Air bubbles on the top could stop the ultrasonic wave and the dump on the bottom decrease and change the ultrasonic entrance angle. Refer to the picture below.

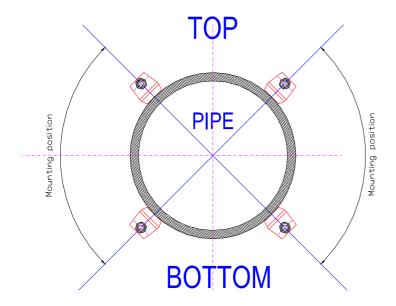


In case of vertical mounting, avoid installing the transducers on downward pipe walls, even if they are under pressure. The pipes with an external lining such as tar, polyethylene, epoxy, should be cleaned when in contact with the transducers.

A tube for acoustic coupling (paste or grease), is included in the supply.


Use a small quantity of coupling grease in order to improve acoustic the contact between the sensor and the pipe's external surface.


2.5.2 "Z" method

Press 1 if you want to choose "Z" mounting.




Press and the device will display:



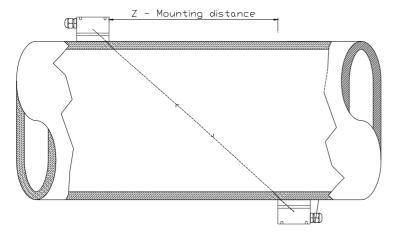


"Z" mounting is more complicated than "V" mounting and it is necessary to create a band of foil as long as the pipe circumference and as wide as indicated in window 25. Additionally, add a piece of paper to wrap the pipe.

Please refer to the picture below for finding the two lines needed to trace the exact half point of the pipe.

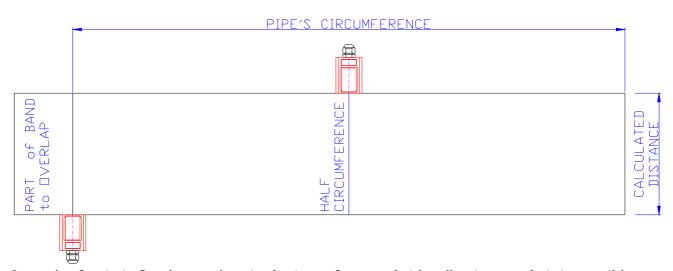

Once the fascia is fixed onto the pipe's circumference (with adhesive tape), it is possible to fix the sensors, as shown in the picture. If the pipe is horizontally mounted, it is suggested

to mount the sensors as shown in the next picture. If the pipe is vertically mounted, refer to the instructions of "V" mounting method.

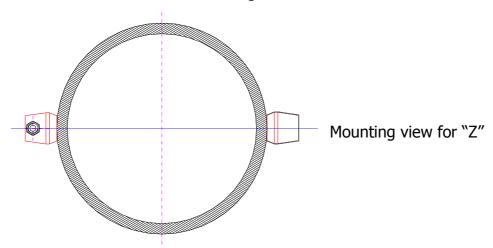

2.5.2 "W" & "N" Mounting Methods


These methods are suitable for small pipes, DN100 or less, with TS-2 transducers.

The signal path consists of four crossings (for "W" method) and three crossings (for "N" method) inside the pipe. These methods are used to increase the transit and receiving time because in other ways the signal path in small pipes will be too short.

In "W" method, the sensors are placed on the same side of the pipe at a definite distance, in "N" method; they are placed on the opposite sides of the pipe, at a definite distance.

These methods are not very used because eve small sensors could be mounted by using "Z" method.

To choose "N" method, press 2 while in menu 24.



Transducer Mounting >0. V

Press and the device will display:

Transducer Mounting

→ 1. Z

Press and the device will display:

Transducer Mounting
>2. N (small pipe)

Press and the device will display:

Transducer Mounting

3. W (small pipe)

Press **ENT**

Transducer Spacing

XXX mm

Press and the device will display:

Default Setting 126
1. Solidify Setting

Press **ENT**

Default Setting [26 >1. Solidify Setting

Press again the device will display:

And the device will display:

Flow 0.0000 m3/h *I Vel 0.0000 m/s

2.5.3 MOUNTING ANALYSIS

After check up the strength of the received signal, total spreading time, time difference and rate of spreading time, we can confirm whether the mounting is suitable.

2.5.4 Signal strength and quality M90



The strength of signals is displayed by numbers from 00.0 to 99.9.

00.0 means no signal received, 99.9 means max signal. In normal working conditions, the signal strength should be bigger than 60.0.

The signal quality (Q) is displayed by numbers from 00.0 to 99.9. 00.0 means the signal is the worst. 99.9 mean signal is the best. In normal working conditions, the signal quality should be bigger than 60.0.

During installation, please pay attention signal strength and quality are at the max level.

2.5.5 Total spreading time, time difference M93


The measurement method is based on time difference, so time and values displayed represent the installation done. In normal operating conditions, the time difference should be smaller that ten percent (10%). If the pipe diameter is small or the speed too low, the difference may be a little bigger. If the difference (and also flow and speed) is too big, it means the signal quality is very bad. The reason may be: pipe's features, unsuitable mounting or wrong parameters setting.

2.5.6 Relation between calculated and measured transit time

To know if the sensors are well mounted, you should calculate:

$$Time _Rate\% = \frac{TOM}{TOS} * 100$$

In normal working conditions it should be 100 +/- 3%.



And eventually confirm the right mounting method.

3 DISPLAY WINDOWS

This chapter will explain all the display windows of TTFM100 Series and their contents. The user can enter this menu by pressing

* [*][*] represent the number of the window to be displayed. The following list includes all the available windows.

3.1 FLOW RATE- TOTALIZERS MENU

- 00 Flow Rate / Net Totalize
- 01 Flow Rate / Velocity
- 02 Flow Rate / POS Totalize
- 03 Flow Rate / NEG Totalize
- 04 Date Time / Flow Rate
- 05 Energy Flow Rate / Totalize
- 06 T1,T2
- 07 AI3, AI4 Input
- 08 System Error Code
- 09 Net Flow Today

3.2 INITIAL SETTING MENU

- 10 Pipe Outer Perimeter
- 11 Pipe Outer Diameter
- 12 Pipe Wall Thickness
- 13 Pipe Inner Diameter
- 14 Pipe Material
- 15 Pipe Sound Velocity
- 16 Liner Material
- (17 Liner Sound Velocity) if in menu 16 the user chooses "other"
- 18 Liner Thickness
- 19 Inside ABS Thickness
- 20 Fluid Type
- (21 Fluid Sound Velocity) if in menu 20 the user chooses "other"
- (22 Fluid Sound Viscosity) if in menu 20 the user chooses "other"
- 23 Transducer Type

Ultrasonic Transit Time Flow meter TTFM100 Series

- 24 Transducer Mounting
- 25 Transducer Spacing
- 26 Default settings
- 27 Save load parameters
- 28 Hold on poor signal
- 29 Empty Pipe Set up

3.3 FLOWRATE UNITS MENU

- 30 Measurement Unit In
- 31 Flow Rate Units
- 32 Totalizer Units
- 33 Totalizer Multiplier
- 34 NET Totalize
- 35 POS Totalize
- 36 NEG Totalize
- 37 Totalizer Reset
- 38 Manual Totalizer
- 39 Language Selection

3.4 OPTIONAL SETTING MENU

- 40 Damping
- 41 Low Flow Cutoff
- 42 Set Zero
- 43 Reset Zero
- 44 Manual Zero Point
- 45 Scale Factor
- 46 Network IDN
- 47 System Lock
- 48 Entry to calibration data
- 49 Serial Port traffic

3.5 INPUTS/ OUTPUTS MENU

- 50 Data Logger Option
- 51 Data Logger Time Setup

Ultrasonic Transit Time Flow meter TTFM100 Series

- 52 Send log data to
- 53 Analog Input AI5
- 54 OCT Pulse width
- 55 CL Mode Select
- 56 CL 4Ma Output Value
- 57 CL 20Ma Output Value
- 58 CL Checkup
- 59 CL Current Output
- 60 Date and Time
- 61 Software Version and ESN
- 62 RS-485 / RS-232 Setup
- 63 Select comm. protocol
- 64 AI3 Value Range
- 65 AI4 Value Range
- 66 AI5 Value Range
- 67 FO Frequency Range
- 68 Low FO Flow Rate
- 69 High FO Flow Rate
- 70 LCD Backlight Option
- 71 LCD Contrast
- 72 Working Timer
- 73 Alarm #1 Low Value
- 74 Alarm #1 High Value
- 75 Alarm #2 Low Value
- 76 Alarm #2 High Value
- 77 Beeper Setup
- 78 OCT Output Setup
- 79 Relay Output Setup
- 80 Batch trigger select
- 81 Flow Batch Controller
- 82 Date Totalizer
- 83 Automatic Amending
- 84 Energy Unit Select
- 85 Temperature Select
- 86 Specific Heat Select
- 87 Energy Totalizer ON/OFF
- 88 Energy Multiplier

89 Differential temperature

3.6 DIAGNOSTICS MENU

- 90 Single Strength and Quality
- 91 TOM / TOS*100
- 92 Fluid Sound Velocity
- 93 Total Time and Delta Time
- 94 Reynolds Number and Factor

3.7 OTHER DISPLAY MENU

From menu 94 onwards, by pressing



It is possible to display some additional information

+ 0	Power ON/OFF Time	+ 5	Calculator
+ 1	Total Work Hours	+ 6	Media velocity Threshold
+ 2	Last Power off Time	+ 7	Total flow for month
+ 3	Last Flow Rate	+ 8	Total flow this year
+ 4	ON/OFF Times	+ 9	Timer

3.8 FLOW RATE - TOTALIZERS MENU ANALYSIS

Digit 0 0 and the device will display

Flow	123.00 m3/h * R
NET	+3452x1m3

This window, display. The scaling units should be set up in menu M31 and M32.

NET is the net totalizer, result of adding the positive totalizer POS to the negative totalizer NEG.

> Digit 10 1 and the device will display

Flow	123.00	m3/h	* R
Vel	0.5678	m/s	

This a display window. The scaling units should be set up in menu M30 and M31.

> Digit 10 2 and the device will display

Ultrasonic Transit Time Flow meter TTFM100 Series

```
Flow 123.00 m3/h * R
POS +3452x1m3
```

This a display window. The scaling units should be set up in menu M3. The POS value refers to the positive totalizer.

> Digit 10 3 and the device will display

```
Flow 123.00 m3/h * R
NEG +0000x1m3
```

This window displays. The scaling units should be set up in menu M31 and M36. The NEG value refers to the negative totalizer.

> Digit 0 4 and the device will display

```
06-08-12 09:54:00 * R
Flow 123.00 m3/h
```

This window displays date and time in the following format yy-mm-dd; hh-mm-ss, and the current flow rate.

Date and time should be set up in menu M60.

This window displays the energy flow and the totalized energy. Pls refer to the part of the manual explaining energy measurements, M84.

> Digit 10 6 and the device will display

```
T1 = 0.0045: -12.456
T2 = 0.0056: -12.547
```

This window displays the analog inputs 1 and 2, respectively: current value and conversion into scaled units.

Digit o 7 and the device will display

```
AI3 = 0.0055: -12.463
AI4 = 0.0058: -12.567
```

This window displays the analog inputs 3 and 4, respectively: current value and conversion into scaled units.

> Digit 10 8 and the device will display



This window displays the error codes. Please refer to the list of complete error codes.

Digit and the device will display

```
Net Flow Today M09
345.34 m3
```

This window displays the net daily flow rate.

3.9 INITIAL SETTING MENU ANALYSIS

> Digit 10 and the device will display

```
Pipe Outer Perimeter
1286 mm
```

This window is used to set up the pipe's perimeter, if known or measurable.

> Digit 1 1 and the device will display

```
Pipe Outer Diameter
409.347 mm
```

This window is used to set up the external pipe's perimeter. When the external perimeter is set up, the external pip's diameter is set up automatically too.

> Digit 1 2 and the device will display

```
Pipe Wall Thickness
6.5 mm
```

This window is used to set up the pipe's thickness. It is also possible to pass over this menu and go to the menu M13, used to set up the internal pipe's diameter.

> Digit 1 3 and the device will display

```
Pipe Inner Diameter
396,347 mm
```

This window is used to set up the net pipe's internal diameter.

> Digit 1 4 and the device will display

```
Pipe Material [14]
0. Carbon Steel
```

This window is used to set up the pipe's material.

Press ENTER to activate the material selection.

Use the arrow keys, () or \(\frac{\frac{1}{1-1}}{1-1} \) or \(\frac{1}{1-1} \) to scroll among the list:

- 0. carbon steel
- 1. stainless steel
- 2. cast iron
- 3. ductile iron
- 4. copper
- 5. PVC
- 6. aluminum
- 7. asbestos
- 8. fiberglass-epoxy
- 9. other

FOR INFORMATION ABOUT THE SOUND SPEED IN OTHER TYPES OF MATERIAL THAT ARE NOT INCLUDED IN THE LIST, PLEASE REFER TO THE TABLES AT PAGES 77 AND 78.

If in you chose "9 – other",

> digit 1 5 and the device will display



Set up the sound speed referring to the construction material of the pipe.

FOR INFORMATION ABOUT THE SOUND SPEED IN OTHER TYPES OF MATERIAL THAT ARE NOT INCLUDED IN THE LIST, PLEASE REFER TO THE TABLES AT PAGES 77 AND 78.

> Digit 10 1 and the device will display

```
Liner Material [16]
0. None, No Liner
```

This window is used to set up the liner's material.

Press ENT to activate the material selection.

Use the arrow keys to scroll among the list:

- 0. no liner
- 1. tar epoxy
- 2. rubber
- 3. mortar
- 4. polypropylene
- 5. polystyrol
- 6. polystyrene

- 7. polyester
- 8. polyethylene
- 9. ebonite
- 10. Teflon
- 11. other

FOR INFORMATION ABOUT THE SOUND SPEED IN OTHER TYPES OF MATERIAL THAT ARE NOT INCLUDED IN THE LIST, PLEASE REFER TO THE TABLES AT PAGES 77 AND 78.

This window will de displayed only if in M16 the user chose "11. OTHER"

> Digit 1 7 and the device will display



Set up the spreading time of sound through the construction material of the liner.

FOR INFORMATION ABOUT THE SOUND SPEED IN OTHER TYPES OF MATERIAL THAT ARE NOT INCLUDED IN THE LIST, PLEASE REFER TO THE TABLES AT PAGES 78 AND 79.

This window will de displayed only if in M16 the user chose "11. OTHER"

➤ Digit and the device will display

```
Liner Thickness [18
0 mm
```

Set up the internal liner thickness,

> Digit 2 0 and the device will display



This window is used to set up the measuring flow type.

Press ENT to enable the fluid selection and use the arrow keys to scroll the list:

- 0. water general
- 1. sea water
- 2. kerosene
- 3. gasoline
- 4. fuel oil
- 5. crude oil
- 6. propane (-45C)
- 7. butane (0C)

- 8. other liquid
- 9. diesel oil
- 10. castor oil
- 11. peanut oil
- 12. gasoline 90
- 13. gasoline 93
- 14. alcohol
- 15. water (125C)

Press ENT to confirm.

This window will de displayed only if in M20 the user chose "8. OTHER LIQUID"

> Digit 2 1 and the device will display

```
Fluid Sound Velocity
1482.8 m/s
```

Set up the spreading time of sound through the fluid to be measured.

FOR INFORMATION ABOUT THE SOUND SPEED IN OTHER TYPES OF MATERIAL THAT ARE NOT INCLUDED IN THE LIST, PLEASE REFER TO THE TABLES FROM PAGE 79 TO PAGE 93.

This window will de displayed only if in M20 the user chose "8. OTHER"

> Digit 2 2 and the device will display

```
Fluid Viscosity [22
1.0038 cST
```

Set up the viscosity of the fluid to be measured.

> Digit 2 3 and the device will display

```
Transducer Type [23]
0. Standard-M
```

This window is used to set up the type of transducers.

Press to enable the transducers type selection and use the arrow keys to scroll the list:

- 0. Standard M
- 1. Insertion type C
- 2. Standard S
- 3. User type
- 4. Standard B
- 5. Insertion B(45)

- 6. Standard L
- 7. JH Polysonics
- 8. Standard HS
- 9. Standard HM
- 10. Standard M1
- 11. Standard S1
- 12. Standard L1
- 13. PI type
- 14. FS410 Fuji
- 15. FS510 Fuji
- 16. Clamp-on TM-1*
- 17. Insertion TC-1
- 18. Clamp-on TS-1*
- 19. Clamp-On TS-2
- 20. Clamp-on TL-1*
- 21. Insertion TLC-2

***OUR STNDARD CLAMP-ON SENSORS**

Press to confirm the type of transducers.

Selection No. 3 "USER TYPE" allows the user to install types of sensors not included in the list. In this case, it is necessary to supply some information about the technical features of the new type of sensors:

1. Wedge degree of ultrasonic impulse.

2. Spreading time through sensor.

3. Distance from crystal to sensor wedge.

4. Delay of ultrasonic signal.

> Digit 2 4 and the device will display

Transducer Mounting
0. V

This window is used to set up the mounting method of the transducers.

Press to enable the transducers type selection and use the arrow keys to scroll the list:

- 0. V
- 1. Z
- 2. N (small pipes)
- 3. W (small pipes)

Press to confirm the type of transducers.

> Digit 2 5 and the device will display

Transducer Spacing
385.268 mm

This window informs about the mounting distance of he transducers. See. Par. 2.4 - 2.5.

> Digit 2 6 and the device will display

Default settings
1. Solidify settings

IMPORTANT: WHEN THE SET-UP PROCEDURE IS COMPLETED, THE USER MUST SELECT THE OPTION:

1. SOLIDIFY SETTINGS

IN THIS WAY THE PARAMETER WILL BE SAVED EVEN IF THE POWER SUPPLY GOES OFF.

> Digit 2 6 and the device will display

Default settings
1. Solidify settings


Press and then use the arrow keys to select among:

Parameters Setup
Use RAM settings

This window allows the loading of one of the 18 saved configurations (from 0 to 17). Press and then use the arrow keys to select the desired configuration, and then select It.:

This window allows displaying one of the 18 configurations saved. Press and use the arrow keys to scroll among the configurations

Press and a new configuration will be saved. Its main feature is:



It refers to the last saved setting. The blinking digit is hiding the number of the setting to be saved (from 0 to 17).

> Digit 2 7 and the device will display

```
Save /Load parameters
123379 mm2
```

This window is used to display the current parameters.

Digit 10 and the device will display

```
Hold on poor signal
YES
```

This window is used to set up the device in order to maintain the last reading as valid in case of temporary loss of signal. If NO is selected, output signal could be modified.

> Digit and the device will display

```
Empty Pipe Setup 129
```

This window is used to set up a min threshold. Below that the device considers the pipe as empty. Set up a value among 30 and 40 in order to be sure the device does not measure when the pipe is empty.

3.10 FLOWRATE UNITS MENU ANALYSIS

> Digit 10 and the it will display

This window is used to set up the measuring system:

- 0. metric
- 1. English

Press and then use the arrow keys to choose the measuring system. Confirm with


➤ Digit 3 1 and the it will display

Flow Rate Units [31 m3/h

This window is used to set up the measuring flow rate units. Press and then use the arrow keys to select the measuring unit among:

- cubic meters
- liters
- US gallon
- UK gallon
- Million US gallon
- Cubic feet
- US oil barrel
- UK oil barrel

Press to confirm the selection and it will display:



Use the arrow keys to select the time units to which the current flow rate should refer:

/hour

/day

/min

/sec

Press to confirm the selection.

Digit 3 2 and the it will display

```
Totalizer Units [32
Cubic Meters (m3)
```

This window is used to set up totalizing flow rate units, please refer to menu M31 for what concerns Volumetric units and their setting.

Factory settings are in m3.

> Digit 3 and the it will display

```
Totalizer Multiplier
3. X1
```

This window is used to set up the multiplying factor for totalization, in order to avoid reaching the max. counting in a short time.

Press and then use the arrow keys to select among:

- 0. X 0.001 (1E-3)
- 1. X 0.01
- 2. X 0.1
- 3. X 1
- 4. X 10
- 5. X 100
- 6. X 1000
- 7. X 10000 (1E+4)

Press **ENT** to confirm.

> Digit (3) 4 and the it will display

```
NET Totalizer [34
ON
```

This window is used to enable the net totalizer, between positive and negative totalizer. Factory setting is ON.

Press and then use the arrow keys to select ON or OFF. Press to confirm.

> Digit 13 5 and the it will display

```
POS Totalizer [35
ON
```

This window is used to enable the positive totalizer. Factory setting is ON.

Press and then use the arrow keys to select ON or OFF. Press to confirm.

> Digit 13 6 and the it will display

```
NEG Totalizer [36
ON
```

This window is used to enable the negative totalizer. Factory setting is ON.

Press and then use the arrow keys to select ON or OFF. Press to confirm.

> Digit 1 and the it will display

```
Totalizer Reset? [37
Selection
```

This window is used to enable the complete or selective zero of internal counters.

Press and then use the arrow keys to select NO or YES. If YES is chosen, please select among:

- 0. no
- 1. yes

Press to confirm the selection and the device will display:

Select Totalizer Reset Finished

> Digit 13 and the it will display

Manual Totalizer [38]
Press ENT When Ready

This window is used to enable the backlog of totalizes. Press to enable the backlog (ON), press again to disable the backlog (OFF).

> Digit 1 and the it will display

Language语言选择 [39 English

This window is used to select the device's display language.

Press and then use the arrow keys to select the language. Press to confirm.

> Digit 4 0 and the it will display

Damping [40

This window allows the user to change the value of damping, the seconds needed to display the analog signals and the output signals. The standard value is between 15 and 30 seconds, the setting range goes from 0 to 99 seconds.

> Digit 4 1 and the it will display

Low Flow Cutoff Val.

0.03 m/s

This window allows the user to set up the speed threshold. Below that level, the device will display 0 flow rate and the totalization is stopped.

> Digit 4 2 and the it will display

Set Zero [42 Press ENT to go

This window is used to enable the flow rate zero procedure with a static fluid. The flow into the pipe must be completely static. The zero procedure has beneficial effects both in low and high flow rate.

Warning!!!

If the flow rate is different from 0, the displayed current flow rate will be 0.

Ultrasonic Transit Time Flow meter TTFM100 Series

Press and the device will display an indicator going right to "0". It will be possible to delete the zero setting by using the next display:

> Digit 4 3 and the it will display

This window is used to delete the zero procedure of the previous menu M42 press and then use the arrow keys to display NO or YES, to disable or enable the deleting function.

> Digit 4 4 and the it will display

This window is used for setting an offset value to be added or detracted (it depends from the setting polarity) to the current flow rate. Usually, if the user knows very well the current flow rate, this function permits to correct the displayed value.

Press and the arrow keys in order to have a negative offset value, followed by the valued to be added or subtract. Press again to confirm.

> Digit 4 5 and the it will display

Scale Factor		[45
	1	

This window is used to set up the scale factor value. This value will affect the measure in order to correct the displayed value.

> Digit 4 6 and the it will display

Network IDN		[46
	88	

This window is used to set up the ID value of the net. The values could be set up aiming 0 and 65535 except for 13(0DH enter), 10(0AH enter), 42(2AH*), 38(26H&), 65535.

The ID value is used during the setting operations to identify the device into a net.

> Digit 4 7 and the it will display

```
System Lock [47

**** Unlocked ****
```

This window is used to set up a password to block the system from unauthorized access. It is composed of a number from 1 up to 4 digits.

> Digit 4 and the it will display

Entry to calibration data [48]
Entry

This window is used to set up the calibration.

> Digit 4 9 and the it will display



This window is used to check the serial port is activated.

3.10.1 INPUTS/ OUTPUTS MENU ANALYSIS

Digit 5 0 and the it will display

This window is used to enable the data logging by using an external logger.

Press and then use , the arrow keys to enable or disable the parameter to be logged.

If ON is chosen, it will be possible to choose among:

- 0. Date and Time
- 1. System Status
- 2. Current Window
- 3. Signal Strength
- 4. Flow Rate
- 5. Velocity
- 6. NET Totalizer
- 7. POS Totalizer
- 8. NEG Totalizer
- 9. Energy Flow Rate
- 10. Energy NET Total
- 11. Energy POS Total
- 12. Energy NEG Total
- 13. Fluid viscosity
- 14. RTD T1
- 15. RTD T2
- 16. Analog Input 3
- 17. analog input 4
- 18. analog input 5

- 19. working timer
- 20. flow today
- 21. serial number

Press and then use the arrow keys to select the desired parameter to be enable/disabled.

> Digit 5 1 and the it will display

This window is used to set up the data logging time.

```
Data Logger Setup [51
Next xx:xx XXXX
```

Press or \(\frac{\frac{1}{2}}{2}\) to go to the following display:

```
Data logger setup
Start Time = 00:00:00
```

This window is used to set up the data logging start time.

Press or to go to the following display:

```
Data logger setup
Interval = 00:00:00
```

This window is used to set up the data logging interval.

Press or \(\frac{\frac{1}{2}}{2}\) to go to the following display:

```
Data logger setup
Log Times = XXXX
```

This window is used to set up the number of Log.

Press and the arrow key to go to the following display:

```
Data Logger Setup [51
Next xx:xx:xx XXXX
```

Warning!!!

The max time interval between two data logging is 24 hours!

Digit 5 2 and the it will display

```
Send log data to [52

→1. Send To RS-485
```

This window cannot be changed from the user. It displays information about the data logging by using the RS485. Refer to chapter 5.

> Digit 5 3 and the it will display

Ultrasonic Transit Time Flow meter TTFM100 Series

Analog Input AI5 53 AI5 = 0.0234 : -24.986

This window displays the status of A15 current input referring to the conversion in measuring units.

> Digit 5 4 and the it will display

This window allows to set up the pulses interval.

This value could be 0....500 mS.

We suggest leaving the factory setting unchanged.

Press to confirm.

> Digit 5 and the it will display

```
CL Mode Select [55]
0. 4 - 20 mA
```

This window is used to set up the current output features (CL= Current Loop). Press and then use the arrow keys to select among:

- 0. 4-20 mA
- 1. 0-20 mA
- 2. 2 0-20 mA via RS485
- 3. 4-20 mA vs fluid
- 4. 20-4-20 mA
- 5. 0-4-20 mA
- 6. 20-0-20 mA
- 7. 4-20 mA vs Velocity
- 8. 4-20mA vs Energy

Press to confirm the selected item.

> Digit 5 6 and the it will display

This window is used to set up the starting range of the output signal for a determined measuring flow rate value. Press and then digit the flow rate starting range value (for example 0 m3/h; if flow rate will be measured in m3). Press again to confirm.

> Digit 5 7 and the it will display

This window is used to set up the ending range of the output signal for a determined measuring flow rate value. Press and then digit the flow rate ending range value (for example 500 m3/h, if flow rate will be measured in m3). Press again to confirm.

> Digit 5 and the it will display

```
CL Checkup [58]
Press ENT When Ready
```

This window allows the simulation of current output in order to check the devices connected to the analog output. Press and then use the arrow keys to select among:

- 0 mA
- 4 mA
- 8 mA
- 12 mA
- 16 mA
- 20 mA

Press again to exit the simulation and the functions in menu M58 will restart.

Warning!!!

HOW COULD THE CURRENT OUTPUT BE CALIBRATED?

Generally, the current outputs is factory set up and calibrate with high precision and rarely is it necessary to change the calibration. If during the simulation M58 the device would measure a value different from the foreseen one, please proceed as follows:

> Digit WEND Y- 0 ENT and the it will display

```
Hardware Adjusting
```

Digit the code 4 2 1 3 0 6 8 and press ent and the device will display:

```
AO Hardware Adjusting M1
Press ENT When Ready
```

Press again and the device will display:

It is suggested to take note of the displayed value (+/-) before changing it. Press the arrow keys and you will be able to change the value, it is also possible to digit it directly. When changed, press again and the device will display:

```
AO Calibration [M.1 20mA = = > 50112
```

It is suggested to take note of the displayed value (+/-) before changing it. Press the arrow keys and you will be able to change the value, it is also possible to digit it directly. When changed, press again and the device will display:

```
AO Hardware Adjusting M.1
Press ENT When Ready
```

The changed value has been saved into the EEPROM (an internal memory which could be deleted only electrically and which keeps the data saved for almost 10 years).

> Digit 2 6 and the device will display

```
Default settings 126
1. Solidify settings
```

IMPORTANT: WHEN THE SET-UP PROCEDURE IS COMPLETED, THE USER MUST SELECT THE OPTION:

1. SOLIDIFY SETTINGS

IN THIS WAY THE PARAMETER WILL BE SAVED EVEN IF THE POWER SUPPLY GOES OFF.

> Digit 5 9 and the device will display

```
CL Current Output [59
4.0000 mA
```

This window is used to display the actual current output, proportional to the measure and to the setting in M55.

> Digit 6 0 and the device will display

```
YY-MM-DD HH:MM:SS
09-10-05 09:54:26
```

This window is used to set up date and time. Press and digit: year, month, day of the month, hour, minute and seconds. Press again to confirm the setting. If during

setting the user makes a mistake, or if it is necessary to change a value, press the key until you reach the desired digit and the digit the right number.

> Digit 6 1 and the device will display



This window displays the software version and the serial number of the device. Due to continuous software updating, the software versions could be different.

> Digit 6 2 and the device will display

```
RS-485 / RS-232 Setup
19200, None
```

This window is used to set up the communication parameters of the serial port. Press and then use the arrow keys to select among:

Baud Rate:

19200

14400

9600

4800

2400

1200

600

300

Press to confirm the selected option and then select the parity type among:

None

Even

Odd

Press to confirm the selection and exit the setting.

The other parameters are factory set up: 8 bit data, 1 bit stop and flow control Xon/Xoff.

> Digit 6 3 and the device will display

```
Select comm protocol

MODBUS ASCII + TDS7
```

This window is used to set up the communication protocol.

Select between:

- MODBUS RTU
- MODBUS ASCII + TDS7
- > Digit 6 4 and the device will display

```
A13 Value Range [64
20 - 100
```

This window is used to set up the conversion into measuring units of 4-20 mA input of analog input 3.

Press and the device will display:

```
AI3 = 4 mA vs. Value
```

Digit the starting range value and press the then press the key and the device will display:

```
AI3 = 20 mA vs. Value
100
```

Digit the ending range value and press the 🔀 key. The setting is finished.

> Digit 6 5 and the device will display

```
AI4 Value Range [65
0 - 100
```

This window is used to set up the conversion into measuring units of 4-20 mA input of analog input 4.

Press and the device will display:

```
AI4 = 4 mA vs. Value
0
```

Digit the starting range value and press (the), then press the () key and the device will display:

Digit the ending range value and press the key. The setting is finished.

> Digit 6 and the device will display

This window is used to set up the conversion into measuring units of 4-20 mA input of analog input 4.

Press and the device will display:

Digit the starting range value and press the then press the key and the device will display:

Digit the ending range value and press the 🔀 key. The setting is finished.

> Digit 6 7 and the device will display

```
FO Frequency Range
0 - 9999
```

This window is used to set up the frequency output in the field 0-9999 Hz, proportionally to the measured flow rate:

Press and key. The device will display:

Digit the starting range value and press (then press the) key and the device will display:

```
High FO Frequency = 9999
```

Digit the ending range value and press the \(\tilde{\tilde

Warning!!!

Use the OCT terminals (open collector) to extract the frequency signal.

> Digit 6 8 and the device will display

This window is used to set up the min. output frequency related to the set up flow rate value.

Press ENT, digit the value in measuring units and press ENT again.

> Digit 6 9 and the device will display

```
High FO Flow Rate 168
500 m3/h
```

This window is used to set up the max output frequency related to the set up flow rate value.

Press ENT, digit the value in measuring units and press ENT again.

> Digit 10 7 0 and the device will display

```
LCD Backlit Option
1. Always ON
```

This window is used to set up the display backlight mode. Press and then use the arrow keys to enter the seconds.

if you select "60" and press ENT, it will display:

```
LCD Backlit Option
60 sec
```

> Digit 1 and the device will display

```
LCD Contrast [71
```

This window is used to set up the display contrast. Press and the use the arrow keys to select a value from 0 up to 31. Press again to confirm the selection.

> Digit 10 7 2 and the device will display

```
Working Timer [72
000000034:54:32
```

This window displays the device working time. Press and then use the arrow keys to delete the device working time. Press to confirm the selection.

> Digit 17 3 and the device will display

```
Alarm #1 Low Value
0 m3/h
```

This window is used to set up the min. flow rate threshold for alarm 1 press ent, digit the flow rate value and press again.

> Digit 7 4 and the device will display

Ultrasonic Transit Time Flow meter TTFM100 Series

This window is used to set up the max flow rate threshold for alarm 1 press (digit the flow rate value and press (again.

> Digit 17 5 and the device will display

This window is used to set up the min. flow rate threshold for alarm 2. press the flow rate value and press again.

> Digit 17 6 and the device will display

This window is used to set up the max flow rate threshold for alarm 1. press (ENT), digit the flow rate value and press (ENT) again.

> Digit 7 7 and the device will display

```
BEEPER Setup [77
16. Not Using
```

This window is used to set up up the buzzer. Press ENT and then use the arrow keys to select among:

- 0. No Signal
- 1. Poor Signal
- 2. Not Ready (No*R)
- 3. Reverse Flow
- 4. AO over 100%
- 5. FO over 120%
- 6. Alarm #1
- 7. Reverse Alarm #2
- 8. Batch Controller
- 9. POS Int Pulse
- 10. NEG Int Pulse
- 11. NET Int Pulse
- 12. Energy POS Pulse
- 13. Energy NEG Pulse
- 14. Energy NET Pulse

- 15. Upper Threshold Velocity
- 16. Lower Threshold Velocity
- 17. ON/OFF via RS485
- 18. Timer (M51 Daily)
- 19. Timed Alarm #1
- 20. Timed Alarm #2
- 21. Batch Total Full
- 22. Timer M51
- 23. batch 90% full
- 24. key stroking on
- 25. disable beeper

Press again to confirm the selection.

> Digit 10 7 8 and the device will display



This window is used to set up the function related to the OCT (open collector) output. Press ENT and then use the arrow keys to select among these options:

- 0. No Signal
- 1. Poor Signal
- 2. Not Ready (No*R)
- 3. Reverse Flow
- 4. AO over 100%
- 5. FO over 120%
- 6. Alarm #1
- 7. Reverse Alarm #2
- 8. Batch Controller
- 9. POS Int Pulse
- 10. NEG Int Pulse
- 11. NET Int Pulse
- 12. Energy POS Pulse
- 13. Energy NEG Pulse
- 14. Energy NET Pulse
- 15. Upper Threshold Velocity
- 16. Lower Threshold Velocity
- 17. ON/OFF via RS485
- 18. Timer (M51 Daily)

- 19. Timed Alarm #1
- 20. Timed Alarm #2
- 21. Batch Total Full
- 22. Timer by M51
- 23. Batch 90% Full
- 24. Flow Rate Pulse
- 25. Disable OCT

Press again to confirm the selection.

> Digit 17 9 and the device will display

RELAY Output Setup
9. POS Int Pulse

This window is used to set up the function related to the relay. Press ENT and then use the arrow keys to select among these options:

- 0. No Signal
- 1. Poor Signal
- 2. Not Ready (No*R)
- 3. Reverse Flow
- 4. AO over 100%
- 5. FO over 120%
- 6. Alarm #1
- 7. Reverse Alarm #2
- 8. Batch Controller
- 9. POS pulse interval
- 10. NEG pulse interval
- 11. NET pulse interval
- 12. Energy POS pulse
- 13. Energy NEG pulse
- 14. Energy NET pulse
- 15. Upper Threshold Velocity
- 16. Lower Threshold Velocity
- 17. ON/OFF via RS485
- 18. Timer (M51 Daily)
- 19. Timed Alarm #1
- 20. Timed Alarm #2
- 21. Batch Total Full
- 22. Timer by M51

- 23. Batch 90% Full
- 24. Disable Relay

Press again to confirm the selection.

Digit 8 0 and the device will display

```
Batch trigger select

0. Key pressing
```

This window is used to set up the function related to the BATCH controller. Press ENT and then use the arrow keys to select one among these options:

- 0. Key Pressing
- 1. Serial Port
- 2. AI3 Rising Edge
- 3. AI3 Falling Edge
- 4. AI4 Rising Edge
- 5. AI4 Falling Edge
- 6. AI5 Rising Edge
- 7. AI5 Falling Edge
- 8. Timer-Periodical
- 9. Timer Daily

Press again to confirm the selection.

Digit 8 1 and the device will display

```
Flow Batch Controller
1000 m3
```

This window is used to set up the volume related to the BATCH function. Press the volume value and press again. The device will display:

```
Flow Batch Controller
```

If in menu M80 you selected "0" key Input, by pressing ENT the device will display:

```
1000 m3
ON 0 m3
```

If ON is blinking, the counter "m3" will increase the value until the BATCH volume is reached. The programmed output for this function will change its status. If you press before reaching the BATCH value, the function will stop.

Digit 8 2 and the device will display

Ultrasonic Transit Time Flow meter TTFM100 Series

Date Totalizer [82 0. browse by day

This window is used to set up the time for logging the flowed volume. Press and then use the arrow keys to select one option among the following:

- 0. browse by day
- 1. browse by month
- 2. browse by year

Press again to confirm the selection and activate the displaying of the following:

The first line display the logging "00" dated 11^{th} of August 2006, other information are related to the current errors, the other line displays the flow rate on the 11^{th} of August 2006 at 23:59:59. press the key to scroll the other 63 loggings. Press to exit this display.

> Digit 8 3 and the device will display

```
Automatic Amending
OFF
```

This window is used to enable the automatic correction of all the totalizer when the device is switched off. The average value (before switching off the device and just after switching on the device) is used to calculate the flowed volume.

Press and then use the arrow keys to display ON or OFF, to enable or disable this function. Press again to confirm the selection.

> Digit 8 4 and the device will display

```
Energy Units Select

0. Giga Joule (GJ)
```

This window is used to select the power measuring units. Press $\stackrel{\text{ENT}}{}$ and then use the $\stackrel{\text{A}/+}{}$ or $\stackrel{\text{V}/-}{}$, to display the following options:

- 0. Giga Joule (GJ)
- 1. Kilocalories (KC)
- 2. KWh
- 3. BTU

Press again to confirm the selection.

Digit 8 5 and the device will display

Temperature Select
0. From T1, T2

This window is used to set up the source for reading the return temperature. Press and then use the arrow keys to display the following options:

- 0. from T1, T2
- 1. from AI3, AI4

Press again to confirm the selection.

> Digit 8 6 and the device will display

Specific Heat Select

1. Fix Specific Heat

This window is used to select the specific heat related into the thermal energy measurement.

Digit 8 7 and the device will display

Energy Totler ON/OFF ON

This window is used to enable the power totalization. Press and the use the arrow keys to display ON or OFF, to enable or to disable this function. Press to confirm the selection.

Digit 8 and the device will display

Energy Multiplier 88
4. x1 (E0)

This window is used to set up the multiplier of the totalization, in order to avoid the reaching of the max counting in a too short time.

- 0. X 0.0001 (E-4)
- 1. X 0.001 (E-3)
- 2. X 0.01 (E-2)
- 3. X 0.1 (E-1)
- 4. X 1 (E0)
- 5. X 10 (E1)
- 6. X 100 (E2)
- 7. X 1000 (E3)
- 8. X 10000 (E4)
- 9. X 100000 (E5)
- 10. X 1000000 (E6)

Press to confirm the selection.

> Digit 18 9 and the device will display

This window is used to set up the temperature differential ΔT .

Press — and the device will display

Set the Heater measurement system:

- 0. Outlet
- 1. Inlet

Press to confirm the selection.

3.11 DIAGNOSTICS MENU ANALYSIS

> Digit 9 0 and the device will display

This window displays the strength and the quality of the signal with numbers from 00.0 to 99.9.

Means that there is no signal, 99.9 mean that the signal is at its max value.

In normal working conditions the strength signal should be around 60.0.

During installation, please pay attention: the quality and strength have to be at their max values.

> Digit 9 1 and the device will display

```
TOM/TOS* 100 [91
100, 25 %
```

This window displays the relationship between the transit time and the measured time. In normal working conditions, it should be 100 + /- 3%. Bigger differences indicate an error in mounting or the setting of wrong parameters.

> Digit 9 2 and the device will display

```
Fluid Sound Velocity
1482.56 m/s
```

This window displays the speed of sound through the fluid. In normal working conditions, the value should be similar to the one indicated in menu M21 big difference indicate an error during the sensors mounting or an error in the setting of M21.

> Digit 9 3 and the device will display

```
Total Time, Delta Time
623,80uS, 242,12nS
```

This window displays the total transit time and the UP-DOWN difference between transit times. The displayed values give information about the installation. In normal working conditions the difference is less than 10%.


If the pipe diameter is small or the fluid velocity is very low, the difference might be a little bigger. If the difference, the flow rate and the speed are too big, they indicate a very bad signal. The causes could be: pipe's features, wrong mounting, wrong parameter setting.

> Digit 9 4 and the device will display

This window displays the calculated Reynolds's number. It indicates the moving mode inside the pipe.

3.12 OTHER DISPLAYS MENU ANALYSIS

> Digit 9 6 and the device will display



The device has been switched ON/OFF in a determined date and time.

Press and then use the arrow keys to display the sequence of 64 events (from 00 up to 63) of switching on and switching off.

Press the 🖅 key to display:

```
Total Work Hours [+1
00000135:34:45
```

Press the 🔨 key to display:

```
Last Power Off Time
06-08-12 09:34:26
```

Press the 🖅 key to display:

```
Last Flow Rate [+3]
0 m3/h
```

Press the 🖅 key to display:

Press the \(\bigsizer\)- key to display:

```
Calculator: Input X = 0
```

It is used as a regular calculator, setting X value, and then Y value. Press to calculate.

Press the 🔀 key to display:

Ultrasonic Transit Time Flow meter TTFM100 Series

Media velocity Threshold
1 m/s

The set up value is used as a threshold to generate an alarm on the relay or on they OCT when it has been passed.

Press the 🔨 key to display:

Total flow for month

Press the 🔀 key to display:

Total flow this year

Press the 📆 key to display:

No-ready timer

4 DIAGNOSTICS AND PROBLEM SOLVING

The TTFM100 series has a complete series of diagnostics functions: it measures and check for errors continuously. The continuous displaying of errors helps the customer identifying damages or unacceptable working conditions.

Displayed errors could happen:

- When switching on the device, during the initial test.
- During functioning, with error codes, in window M108.

Causes and solutions are indicated in the below following table:

4.1 AUTOTEST DURING SWITCHING ON AND POSSIBLE SOLUTIONS

ERROR DESCRIPTION	SOLUTIONS		
ROM PARITY ERROR	Contact B.M. Tecnologie Industriali.		
STORED DATA ERROR	Digit ENT again during the initial set up up.		
HAND SHAKING ERR =*	Switch off and then switch on.		
CPU FATAL ERROR	Contact B.M. Tecnologie Industriali.		
TIMER SLOW ERROR TIMER FAST ERROR	Switch off and then switch on or contact B.M. Tecnologie Industriali.		
SYSTEM RAM ERROR	Switch off and then switch on or contact B.M. Tecnologie Industriali.		
TIME OR BATT ERROR	Switch off and then switch on or contact B.M. Tecnologie Industriali.		
LCD TIMEOVER ERROR	Check the display or the electronics connections.		
PRN TIME OVER	Check the printer or the connections.		

4.2 ERROR CODES, CAUSES AND SOLUTIONS DURING FUNCTIONING

ERROR CODE	INFORMATION IN M08 WINDOW	CAUSES	SOLUTIONS
*R	Normal system	Regular functioning	
*]	Sub CPU wrong	Damage in sub CPU	Contact B.M. Tecnologie Industriali.
*I	No signal detected	No signal detected: - sensor far from the pipe or not so coupling - wrong sensors mounting - too many oxide or dump inside the pipe - new linearity	 check the acoustic contact with the pipe's surface. use another coupling grease check initial settings try to reduce the pipe's internal dumps or change the sensors position wait for stable linearity.
*H	Low strength signal	Low signal strength	SEE ABOVE
*H	Poor quality signal	Poor signal quality	SEE ABOVE
*Q	Freq output power	Output frequency bigger than 120%, very high flow rate or wrong settings.	Check again the settings in M66 and in M69 or simply confirm that the flow rate should be so big.
*E	Over current loop	Output current bigger than 100%, very high flow rate or wrong settings.	Check again the settings in M66 or simply confirm that the flow rate should be so big.
*F	Ref. to table 1	Please find the problem during initial test. Switch off and then on or contact Tecnologie Industriali	
*G	ADJ GAIN= S1 ADJ GAIN= S2 ADJ GAIN= S3 ADJ GAIN= S4	THE DEVICE IS DOING THE AUTOTEST REGULATIONS.	

5 COMMUNICATION WITH A PC AND/ OR DATA LOGGING

This chapter informs the user about the hardware connections to be done to allow a communication between the device and the PC.

5.1 DIRECT CONTROLS - PROTOCOL

The following controls are also used by the Transit Time Flow meter FUJI-FLV, here used as a reference.

NOTE: IT IS NECESSARY TO BEGIN A NEW LINE WITH (CR) CONTROL.

CONTROL	DATA TRANSMISS	SION	CONTROL	DATA TRANSMISSION
DQD (CR)	DAILY TRANSMISSION	FLOWRATE	M@(CR)	SIMULATION OF THE CODE SENT TO THE TTFM100
DQH(CR)	HOUR TRANSMISSION	FLOWRATE	LCD(CR)	TRASNMISSION TO THE DISPLAY
DQM(CR)	MINUTE TRANSMISSION	FLOWRATE	C1(CR)	OCT OUTPUT ON
DQS(CR)	SECOND TRANSMISSION	FLOWRATE	C0(CR)	OCT OUTPUT OFF
DV(CR)	FLOWRATE TRANSMISSION	SPEED	R1(CR)	RELAY OUTPUT ON
DI+(CR)	POSITIVE TRANSMISSION	TOTALIZER	R0(CR)	RELAY OUTPUT OFF
DI-(CR)	NEGATIVE TRANSMISSION	TOTALIZER	F0n8cr)	FREQUENCE OUTPUT CONTROL AS A "n" VALUE
DIN(CR)	NET TRANSMISSION	TOTALIZER	A0a(CR)	CURRENT OUTPUT CONTROL AS AN "a" VALUE
DIE(CR)	ENERGY TRANSMISSION	TOTALIZER	BA1(CR)	THE BINARY VALUE OF AI1 INPUT RETURNS
DL(CR)	SIGNAL TRANSMISSION	STRENGTH	BA2(CR)	THE BINARY VALUE OF AI2 INPUT RETURNS
DS(CR)	THE PERCENTAGE OUTPUT SIGNAL RE		AI1(CR)	THE VALUE OF INSTANTANEOUS INPUT AI1 RETURNS
DC(CR)	ERROR CODES REQ	UEST	AI2(CR)	THE VALUE OF INSTANTANEOUS INPUT AI2

Ultrasonic Transit Time Flow meter TTFM100 Series

			RETURNS
DA(CR)	OCT OR RELAY ALARMS	ESN	DEVICE SERIAL NUMBER
DT(CR)	CURRENT DATE AND TIME		

6 APPENDIX

6.1 SOUND SPEEDS IN SOLIDS

Table 1: Sound Speeds in Solids

Table 1. Sc	Sound	Speed* ive (25°C)	Sound	Speed* ve (25°C)	
Material	m/s	ft/s	mm/µs	in./µs	
Steel, 1% Carbon, hardened	3,150	10,335	5.88	0.2315	
Carbon Steel	3,230	10,598	5.89	0.2319	
Mild Steel	3,235	10,614	5.89	0.2319	
Steel, 1% Carbon	3,220	10,565			
302 Stainless Steel	3,120	10,236	5.690	0.224	
303 Stainless Steel	3,120	10,236	5.640	0.222	
304 Stainless Steel	3,141	10,306	5.920	0.233	
304L Stainless Steel	3,070	10,073	5.790	0.228	
316 Stainless Steel	3,272	10,735	5.720	0.225	
347 Stainless Steel	3,095	10,512	5.720	0.225	
Aluminum	3,100	10,171	6.32	0.2488	
Aluminum (rolled)	3,040	9,974			
Copper	2,260	7,415	4.66	0.1835	
Copper (annealed)	2,325	7,628			
Copper (rolled)	2,270	7,448			
CuNi (70%Cu 30%Ni)	2,540	8,334	5.03	0.1980	
CuNi (90%Cu 10%Ni)	2,060	6,759	4.01	0.1579	
Brass (Naval)	2,120	6,923	4.43	0.1744	
Gold (hard-drawn)	1,200	3,937	3.24	0.1276	
Inconel	3,020	9,909	5.82	0.2291	
Iron (electrolytic)	3,240	10,630	5.90	0.2323	
Iron (Arm∞)	3,240	10,630	5.90	0.2323	

^{*}Please note these values are to be considered nominal. Solids may be inhomogenous and anisotropic. Actual values depend on exact composition, temperature, and to a lesser extent, on pressure or stress.

Table 1: Sound Speeds in Solids (cont.)

Table 1. South	Sound	Speed* ive (25°C)	Sound	Speed* ive (25°C)
Material	m/s	(ft/s)	mm/μs	in/μs
Ductile Iron	3,000	9,843		
Cast Iron	2,500	8,203	4.55	0.1791
Monel	2,720	8,924	5.35	0.2106
Nickel	2,960	9,712	5.63	0.2217
Tin, rolled	1,670	5,479	3.32	0.1307
Titanium	3,125	10,253	6.10	0.2402
Tungsten, annealed	2,890	9,482	5.18	0.2039
Tungsten, drawn	2,640	8,661		
Tungsten, carbide	3,980	13,058		
Zinc, rolled	2,440	8,005	4.17	0.1642
Glass, Pyrex	3,280	10,761	5.61	0.2209
Glass, heavy silicate flint	2,380	7,808		
Glass, light borate crown	2,840	9,318	5.26	0.2071
Nylon	1,150	3,772	2.40	0.0945
Nylon, 6-6	1,070	3,510		
Polyethylene (HD)			2.31	0.0909
Polyethylene (LD)	540	1,772	1.94	0.0764
PVC, CPVC	1,060	3,477	2.40	0.0945
Acrylic	1,430	4,690	2.73	0.1075
Asbestos Cement			2.20	0.0866
Tar Epoxy			2.00	0.0787
Mortar			2.50	0.0984
Rubber			1.90	0.0748

^{*}Please note these values are to be considered nominal. Solids may be inhomogenous and anisotropic. Actual values depend on exact composition, temperature, and to a lesser extent, on pressure or stress.

6.2 SOUND SPEEDS IN FLUIDS

Table 2: Sound Speeds in Fluids

		All data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	Δ v /°C	Kinematic Viscosity x10 ⁻⁶	
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Acetic anhydride (22)	(CH ₃ CO) ₂ O	1.082 (20°C)	1,180	3,871.4	2.5	0.769	8.274
Acetic acid, anhydride (22)	(CH ₃ CO) ₂ O	1.082 (20°C)	1,180	3,871.4	2.5	0.769	8.274
Acetic acid, nitrile	C₂H₃N	0.783	1,290	4,232.3	4.1	0.441	4.745
Acetic acid, ethyl ester (33)	C ₄ H ₈ O ₂	0.901	1,085	3,559.7	4.4	0.467	5.025
Acetic acid, methyl ester	C ₃ H ₆ O ₂	0.934	1,211	3,973.1		0.407	4.379
Acetone	C ₃ H ₆ O	0.791	1,174	3,851.7	4.5	0.399	4.293
Acetonitrile	C ₂ H ₃ N	0.783	1,290	4,232.3	4.1	0.441	4.745
Acetonylacetone	C ₆ H ₁₀ O ₂	0.729	1,399	4,589.9	3.6		
Acetylen dichloride	C ₂ H ₂ Cl ₂	1.26	1,015	3,330.1	3.8	0.400	4.304
Acetylene tetrabromide (47)	C ₂ H ₂ Br ₄	2.966	1,027	3,369.4			
Acetylene tetrachloride (47)	C₂H₂Cl₄	1.595	1,147	3,763.1		1.156 (15°C)	12.438 (59°F)
Alcohol	C ₂ H ₆ O	0.789	1,207	3,960	4.0	1.396	15.02
Alkazene-13	C ₁₅ H ₂₄	0.86	1,317	4,320.9	3.9		
Alkazene-25	C ₁₀ H ₁₂ Cl ₂	1.20	1,307	4,288.1	3.4		
2-Amino-ethanol	C ₂ H ₇ NO	1.018	1,724	5,656.2	3.4		
2-Aminotolidine (46)	C ₇ HgN	0.999 (20°C)	1,618	5,308.4		4.394 (20°C)	47.279 (68°F)
4-Aminotolidine (46)	C ₇ HgN	0.966 (45°C)	1,480	4,855.6		1.863 (50°C)	20.045 (122°F)
Ammonia (35)	NH ₃	0.771	1,729 (-33°C)	5,672.6 (-27°F)	6.68	0.292 (-33°C)	3.141 (-27°F)
Amorphous Polyolefin		0.98	962.6 (190°C)	3158.2 (374°F)		26,600	286,000
t-Amyl alcohol	C ₅ H ₁₂ O	0.81	1,204	3,950.1		4.374	47.064
Aminobenzene (41)	C ₆ H ₅ NO ₂	1.022	1,639	5,377.3	4.0	3.63	39.058
Aniline (41)	C ₆ H ₅ NO ₂	1.022	1,639	5,377.3	4.0	3.63	39.058
Argon (45)	Ar	1.400 (-188°C)	853 (-188°C)	2798.6 (-306°F)			

Table 2: Sound Speeds in Fluids (cont.)

		Ali data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	_	Speed			matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Azine	C ⁶ H ^a N	0.982	1,415	4,642.4	4.1	0.992 (20°C)	10.673 (68°F)
Benzene (29, 40, 41)	C ₆ H ₆	0.879	1,306	4,284.8	4.65	0.711	7.65
Benzol (29, 40, 41)	C ₆ H ₆	0.879	1,306	4,284.8	4.65	0.711	7.65
Bromine (21)	Br ₂	2.928	889	2,916.7	3.0	0.323	3.475
Bromo-benzene (46)	C ₆ H ₅ Br	1.522	1,170 (20°C)	3,838.6 (68°F)		0.693	7.456
1-Bromo-butane (46)	C ₄ H ₉ Br	1.276 (20°C)	1,019 (20°C)	3,343.2 (68°F)		0.49 (15°C)	5.272 (59°F)
Bromo-ethane (46)	C₂H₅Br	1.460 (20°C)	900 (20°C)	2,952.8 (68°F)		0.275	2.959
Bromoform (46, 47)	CHBr ₃	2.89 (20°C)	918	3,011.8	3.1	0.654	7.037
n-Butane (2)	C ₄ H ₁₀	0.601 (0°C)	1,085 (-5°C)	3,559.7 (23°F)	5.8		
2-Butanol	C ₄ H ₁₀ O	0.81	1,240	4,068.2	3.3	3.239	34.851
sec-Butylalcohol	C ₄ H ₁₀ O	0.81	1,240	4,068.2	3.3	3.239	34.851
n-Butyl bromide (46)	C ₄ H ₉ Br	1.276 (20°C)	1,019 (20°C)	3,343.2 (68°F)		0.49 (15°C)	5.272 (59°F)
n-Butyl chloride (22, 46)	C ₄ H ₉ CI	0.887	1,140	3,740.2	4.57	0.529 (15°C)	5.692 (59°F)
tert Butyl chloride	C ₄ H ₉ CI	0.84	984	3,228.3	4.2	0.646	6.95
Butyl oleate	C ₂₂ H ₄₂ O ₂		1,404	4,606.3	3.0		
2, 3 Butylene glycol	C ₄ H ₁₀ O ₂	1.019	1,484	4,868.8	1.51		
Cadmium (7)	Cd		2,237.7 (400°C)	7,341.5 (752°F)		1.355cp (440°C)	14.579 (824°F)
Carbinol (40, 41)	CH ₄ O	0.791 (20°C)	1,076	3,530.2	2.92	0.695	7.478
Carbitol	C ₆ H ₁₄ O ₃	0.988	1,458	4,783.5			
Carbon dioxide (26)	CO ₂	1.101 (-37°C)	839 (-37°C)	2,752.6 (-35°F)	7.71	0.137 (-37°C)	1.474 (-35°F)
Carbon disulphide	CS ₂	1.261 (22°C)	1,149	3,769.7		0.278	2.991

Table 2: Sound Speeds in Fluids (cont.)

		All data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	∆v/°C	Kinematic Viscosity x10 ⁻⁶	
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Carbon tetrachloride (33, 35, 47)	CCI ₄	1.595 (20°C)	926	3038.1	2.48	0.607	6.531
Carbon tetrafluoride (14) (Freon 14)	CF ₄	1.75 (-150°C)	875.2 (-150°C)	2,871.5 (-238°F)	6.61		
Cetane (23)	C ₁₆ H ₃₄	0.773 (20°C)	1,338	4,389.8	3.71	4.32	46.483
Chloro-benezene	C ₆ H ₅ CI	1.106	1,273	4,176.5	3.6	0.722	7.768
1-Chloro-butane (22, 46)	C₄H ₉ CI	0.887	1,140	3,740.2	4.57	0.529 (15°C)	5.692 (59°F)
Chloro-diFluoromethane (3) (Freon 22)	CHCIF ₂	1.491 (-69°C)	893.9 (-50°C)	2,932.7 (-58°F)	4.79		
Chloroform (47)	CHCl₃	1.489	979	3,211.9	3.4	0.55	5.918
1-Chloro-propane (47)	C ₃ H ₇ CI	0.892	1,058	3,471.1		0.378	4.067
Chlorotrifluoromethane (5)	CCIF ₃		724 (-82°C)	2,375.3 (-116°F)	5.26		
Cinnamaldehyde	C ₉ H ₈ O	1.112	1,554	5,098.4	3.2		
Cinnamic aldehyde	C ₉ H ₈ O	1.112	1,554	5,098.4	3.2		
Colamine	C ₂ H ₇ NO	1.018	1,724	5,656.2	3.4		
o-Cresol (46)	C ₇ H ₈ O	1.047 (20°C)	1,541 (20°C)	5,055.8 (68°F)		4.29 (40°C)	46.16 (104°F)
m-Cresol (46)	C ₇ H ₈ O	1.034 (20°C)	1,500 (20°C)	4,921.3 (68°F)		5.979 (40°C)	64.334 (104°F)
Cyanomethane	C ₂ H ₃ N	0.783	1,290	4,232.3	4.1	0.441	4.745
Cyclohexane (15)	C ₆ H ₁₂	0.779 (20°C)	1,248	4,094.5	5.41	1.31 (17°C)	14.095 (63°F)
Cyclohexanol	C ₆ H ₁₂ O	0.962	1,454	4,770.3	3.6	0.071 (17°C)	0.764 (63°F)
Cyclohexanone	C ₆ H ₁₀ O	0.948	1,423	4,668.6	4.0		
Decane (46)	C ₁₀ H ₂₂	0.730	1,252	4,107.6		1.26 (20°C)	13.55 (68°F)
1-Decene (27)	C ₁₀ H ₂₀	0.746	1,235	4,051.8	4.0		
n-Decylene (27)	C ₁₀ H ₂₀	0.746	1,235	4,051.8	4.0		
Diacetyl	C ₄ H ₆ O ₂	0.99	1,236	4,055.1	4.6		

Table 2: Sound Speeds in Fluids (cont.)

		All data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	∆v/°C		matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Diamylamine	C ₁₀ H ₂₃ N		1,256	4,120.7	3.9		
1,2 Dibromo-ethane (47)	C ₂ H ₄ Br ₂	2.18	995	3,264.4		0.79 (20°C)	8.5 (68°F)
trans-1,2-Dibromoethene (47)	C ₂ H ₂ Br ₂	2.231	935	3,067.6			
Dibutyl phthalate	C ₈ H ₂₂ O ₄		1,408	4,619.4			
Dichloro-t-butyl alcohol	C ₄ H ₈ Cl ₂ O		1,304	4,278.2	3.8		
2,3 Dichlorodioxane	C ₂ H ₆ Cl ₂ O ₂		1,391	4,563.6	3.7		
Dichlorodifluoromethane (3) (Freon 12)	CCl ₂ F ₂	1.516 (40°C)	774.1	2,539.7	4.24		
1,2 Dichloro ethane (47)	C ₂ H ₄ Cl ₂	1.253	1,193	3,914		0.61	6.563
cis1,2-Dichloro-ethene (3, 47)	C ₂ H ₂ Cl ₂	1.284	1,061	3,481			
trans1,2-Dichloro-ethene (3, 47)	C ₂ H ₂ Cl ₂	1.257	1,010	3,313.6			
Dichloro-fluoromethane (3) (Freon 21)	CHCl₂F	1.426 (0°C)	891 (0°C)	2,923.2 (32°F)	3.97		
1-2-Dichlorohexafluoro- cyclobutane (47)	C ₄ Cl ₂ F ₆	1.654	669	2,194.9			
1-3-Dichloro-isobutane	C ₄ H ₈ Cl ₂	1.14	1,220	4,002.6	3.4		
Dichloro methane (3)	CH ₂ CI ₂	1.327	1,070	3,510.5	3.94	0.31	3.335
1,1-Dichloro-1,2,2,2 tetra fluoroethane	CCIF ₂ CCIF ₂	1.455	665.3 (-10°C)	2,182.7 (14°F)	3.73		
Diethyl ether	C ₄ H ₁₀ O	0.713	985	3,231.6	4.87	0.311	3.346
Diethylene glycol	C ₄ H ₁₀ O ₃	1.116	1,586	5,203.4	2.4		
Diethylene glycol, monoethyl ether	C ₆ H ₁₄ O ₃	0.988	1,458	4,783.5			
Diethylenimide oxide	C ₄ H ₉ NO	1.00	1,442	4,731	3.8		
1,2-bis(DiFluoramino) butane (43)	C ₄ H ₈ (NF ₂) ₂	1.216	1,000	3,280.8			
1,2-bis(DiFluoramino)- 2-methylpropane (43)	C ₄ H ₉ (NF ₂) ₂	1.213	900	2,952.8			
1,2-bis(DiFluoramino) propane (43)	C ₃ H ₆ (NF ₂) ₂	1.265	960	3,149.6			

Table 2: Sound Speeds in Fluids (cont.)

		All data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	∆v/°C	Kine Viscosi	matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
2,2-bis(DiFluoramino propane (43)	C ₃ H ₆ (NF ₂) ₂	1.254	890	2920			
2,2-Dihydroxydiethyl ether	C ₄ H ₁₈ O ₃	1.116	1,586	5,203.4	2.4		
Dihydroxyethane	C ₂ H ₆ O ₂	1.113	1,658	5,439.6	2.1		
1,3-Dimethyl-benzene (46)	C ₈ H ₁₀	0.868 (15°C)	1,343 (20°C)	4,406.2 (68°F)		0.749 (15°C)	8.059 (59°F)
1,2-Dimethyl-benzene (29, 46)	C ₈ H ₁₀	0.897 (20°C)	1,331.5	4,368.4	4.1	0.903 (20°C)	9.716 (68°F)
1,4-Dimethyl-benzene (46)	C ₈ H ₁₀		1,334 (20°C)	4,376.6 (68°F)		0.662	7.123
2,2-Dimethyl-butane (29, 33)	C ₆ H ₁₄	0.649 (20°C)	1,079	3,540			
Dimethyl ketone	C ₃ H ₆ O	0.791	1,174	3,851.7	4.5	0.399	4.293
Dimethyl pentane (47)	C ₇ H ₁₆	0.674	1,063	3,487.5			
Dimethyl phthalate	C ₈ H ₁₀ O ₄	1.2	1,463	4,799.9			
Diiodo-methane	CH ₂ l ₂	3.235	980	3,215.2			
Dioxane	C ₄ H ₈ O ₂	1.033	1,376	4,514.4			
Dodecane (23)	C ₁₂ H ₂₆	0.749	1,279	4,196.2	3.85	1.80	19.368
1,2-Etha nediol	C ₂ H ₆ O ₂	1.113	1,658	5,439.6	2.1		
Ethanenitrile	C₂H₃N	0.783	1,290	4,232.3		0.441	4.745
Ethanoic anhydride (22)	(CH ₃ CO) ₂ O	1.082	1,180	3,871.4		0.769	8.274
Ethanol	C ₂ H ₆ O	0.789	1,207	3,960	4.0	1.39	14.956
Ethanol amide	C ₂ H ₇ NO	1.018	1,724	5,656.2	3.4		
Ethoxyethane	C ₄ H ₁₀ O	0.713	985	3,231.6	4.87	0.311	3.346
Ethyl acetate (33)	C ₄ H ₈ O ₂	0.901	1,085	3,559.7	4.4	0.489	5.263
Ethyl alcohol	C ₂ H ₆ O	0.789	1,207	3,960	4.0	1.396	15.020
Ethyl benzene (46)	C ₈ H ₁₀	0.867 (20°C)	1,338 (20°C)	4,389.8 (68°F)		0.797 (17°C)	8.575 (63°F)
Ethyl Bromide (46)	C ₂ H ₅ Br	1.461 (20°C)	900 (20°C)	2,952.8 (68°F)		0.275 (20°C)	2.959 (68°F)
Ethyliodide (46)	C ₂ H ₅ I	1.950 (20°C)	876 (20°C)	2874 (68°F)		0.29	3.12

Table 2: Sound Speeds in Fluids (cont.)

		Ali data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	Δ v /°C		matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Ether	C ₄ H ₁₀ O	0.713	985	3231.6	4.87	0.311	3.346
Ethyl ether	C ₄ H ₁₀ O	0.713	985	3231.6	4.87	0.311	3.346
Ethylene bromide (47)	C ₂ H ₄ Br ₂	2.18	995	3264.4		0.79	8.5
Ethylene chloride (47)	C ₂ H ₄ Cl ₂	1.253	1,193	3914		0.61	6.563
Ethylene glycol	C ₂ H ₆ O ₂	1.113	1,658	5439.6	2.1	17.208 (20°C)	185.158 (68°F)
d-Fenochone	C ₁₀ H ₁₆ O	0.947	1,320	4330.7		0.22	2.367
d-2-Fenedhanone	C ₁₀ H ₁₆ O	0.947	1,320	4330.7		0.22	2.367
Fluorine	F	0.545 (-143°C)	403 (-143°C)	1322.2 (-225°F)	11.31		
Fluoro-benzene (46)	C ₆ H₅F	1.024 (20°C)	1,189	3900.9		0.584 (20°C)	6.283 (68°F)
Formaldehyde, methyl ester	C ₂ H ₄ O ₂	0.974	1,127	3697.5	4.02		
Formamide	CH ₃ NO	1.134 (20°C)	1,622	5321.5	2.2	2.91	31.311
Formic acid, amide	CH ₃ NO	1.134 (20°C)	1,622	5321.5		2.91	31.311
Freon R12			774.2	2540			
Furfural	C ₅ H ₄ O ₂	1.157	1,444	4737.5	3.7		
Furfuryl alcohol	C ₅ H ₆ O ₂	1.135	1,450	4757.2	3.4		
Fural	C ₅ H ₄ O ₂	1.157	1,444	4737.5	3.7		
2-Furaldehyde	C ₅ H ₄ O ₂	1.157	1,444	4737.5	3.7		
2-Furancarboxaldehyde	C ₅ H ₄ O ₂	1.157	1,444	4737.5	3.7		
2-Furyl-Methanol	C₅H ₆ O ₂	1.135	1,450	4757.2	3.4		
Gallium	Ga	6.095	2,870 (30°C)	9416 (86°F)			
Glycerin	C ₃ H ₈ O ₃	1.26	1,904	6246.7	2.2	757.1	8,081.836
Glycerol	C ₃ H ₈ O ₃	1.26	1,904	6246.7	2.2	757.1	8,081.836
Glycol	C ₂ H ₆ O ₂	1.113	1658	5439.6	2.1		
50% Glycol / 50% H ₂ O			1,578	5,177			

Table 2: Sound Speeds in Fluids (cont.)

		Ali data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	Δ v /°C	Kinematic Viscosity x10 ⁻⁶	
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Helium (45)	He ₄	0.125 (-269°C)	183 (-269°C)	600.4 (-452°F)		0.025	.269
Heptane (22, 23)	C ₇ H ₁₆	0.684 (20°C)	1,131	3,710.6	4.25	0.598 (20°C)	6.434 (68°F)
n-Heptane (29, 33)	C ₇ H ₁₆	0.684 (20°C)	1,180	3,871.3	4.0		
Hexachloro- Cydopentadiene (47)	C₅Cl ₆	1.7180	1,150	3,773			
Hexadecane (23)	C ₁₆ H ₃₄	0.773 (20°C)	1,338	4,389.8	3.71	4.32 (20°C)	46.483 (68°F)
Hexalin	C ₆ H ₁₂ O	0.962	1,454	4,770.3	3.6	70.69 (17°C)	760.882 (63°F)
Hexane (16, 22, 23)	C ₆ H ₁₄	0.659	1,112	3,648.3	2.71	0.446	4.798
n-Hexane (29, 33)	C ₆ H ₁₄	0.649 (20°C)	1,079	3,540	4.53		
2,5-Hexanedione	C ₆ H ₁₀ O ₂	0.729	1,399	4,589.9	3.6		
n-Hexanol	C ₆ H ₁₄ O	0.819	1,300	4,265.1	3.8		
Hexahydrobenzene (15)	C ₆ H ₁₂	0.779	1,248	4,094.5	5.41	1.31 (17°C)	14.095 (63°F)
Hexahydrophenol	C ₆ H ₁₂ O	0.962	1,454	4,770.3	3.6		
Hexamethylene (15)	C ₆ H ₁₂	0.779	1,248	4,094.5	5.41	1.31 (17°C)	14.095 (63°F)
Hydrogen (45)	H ₂	0.071 (-256°C)	1,187 (-256°C)	3,894.4 (-429°F)		0.003 (-256°C)	0.032 (-429°F)
2-Hydroxy-toluene (46)	C ₇ H ₈ O	1.047 (20°C)	1,541 (20°C)	5,055.8 (68°F)		4.29 (40°C)	46.16 (104°F)
3-Hydroxy-toluene (46)	C ₇ H ₈ O	1.034 (20°C)	1,500 (20°C)	4,921.3 (68°F)		5.979 (40°C)	64.334 (104°F)
lodo-benzene (46)	C ₆ H ₅ I	1.823	1,114 (20°C)	3,654.9 (68°F)		0.954	
lodo-ethane (46)	C₂H₅I	1.950 (20°C)	876 (20°C)	2,874 (68°F)		0.29	3.12
lodo-methane	CH ₃ I	2.28 (20°C)	978	3,208.7		0.211	2.27
Isobutyl acetate (22)	C ₆ H ₁₂ O		1,180 (27°C)	3,871.4 (81°F)	4.85		

Table 2: Sound Speeds in Fluids (cont.)

		All data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	Δ v /°C		matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Isobutanol	C ₄ H ₁₀ O	0.81 (20°C)	1,212	3,976.4			
Iso-Butane			1,219.8	4002			
Isopentane (36)	C ₅ H ₁₂	0.62 (20°C)	980	3,215.2	4.8	0.34	3.658
Isopropanol (46)	C ₃ H ₈ O	0.785 (20°C)	1,170 (20°C)	3,838.6 (68°F)		2.718	29.245
Isopropyl alcohol (46)	C ₃ H ₈ O	0.785 (20°C)	1,170 (20°C)	3,838.6 (68°F)		2.718	29.245
Kerosene		0.81	1,324	4,343.8	3.6		
Ketohexamethylene	C ₆ H ₁₀ O	0.948	1,423	4,668.6	4.0		
Lithium fluoride (42)	LiF		2,485 (900°C)	8,152.9 (1652°F)	1.29		
Mercury (45)	Hg	13.594	1,449 (24°C)	4,753.9 (75°F)		0.114	1.226
Mesityloxide	C ₆ H ₁₆ O	0.85	1,310	4,297.9			
Methane (25, 28, 38, 39)	CH₄	0.162 (-89°C)	405 (-89°C)	1,328.7 (-128°F)	17.5		
Methanol (40, 41)	CH ₄ O	0.791 (20°C)	1,076	3,530.2	2.92	0.695	7.478
Methyl acetate	C ₃ H ₆ O ₂	0.934	1,211	3,973.1		0.407	4.379
o-Methylaniline (46)	C ₇ H ₉ N	0.999 (20°C)	1,618	5,308.4		4.394 (20°C)	47.279 (68°F)
4-Methylaniline (46)	C ₇ HgN	0.966 (45°C)	1,480	4,855.6		1.863 (50°C)	20.095 (122°F)
Methyl alcohol (40, 44)	CH ₄ O	0.791 (20°C)	1,076	3,530.2	2.92	0.695	7.478
Methyl benzene (16, 52)	C ₇ H ₈	0.867	1,328 (20°C)	4,357 (68°F)	4.27	0.644	7.144
2-Methyl-butane (36)	C₅H ₁₂	0.62 (20°C)	980	3,215.2		0.34	3.658
Methyl carbinol	C ₂ H ₆ O	0.789	1,207	3,960	4.0	1.396	
Methyl-chloroform (47)	C ₂ H ₃ Cl ₃	1.33	985	3,231.6		0.902 (20°C)	9.705 (68°F)
Methyl-cyanide	C₂H₃N	0.783	1,290	4,232.3		0.441	4.745

Table 2: Sound Speeds in Fluids (cont.)

		-	given at 2	•		otherwise	noted.
Substance	Chemical	Specific	_	Speed	Δv/°C	Kine	matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
3-Methyl cyclohexanol	C ₇ H ₁₄ O	0.92	1,400	4,593.2			
Methylene chloride (3)	CH ₂ Cl ₂	1.327	1,070	3,510.5	3.94	0.31	3.335
Methylene iodide	CH ₂ I ₂	3.235	980	3,215.2			
Methyl formate (22)	C ₂ H ₄ O ₂	0.974 (20°C)	1,127	3,697.5	4.02		
Methyl iodide	CH ₃ I	2.28 (20°C)	978	3,208.7		0.211	2.27
a-Methyl naphthalene	C ₁₁ H ₁₀	1.090	1,510	4,954.1	3.7		
2-Methylphenol (46)	C ₇ H ₈ O	1.047 (20°C)	1,541 (20°C)	5,055.8 (68°F)		4.29 (40°C)	46.16 (104°F)
3-Methylphenol (46)	C ₇ H ₈ O	1.034 (20°C)	1,500 (20°C)	4,921.3 (68°F)		5.979 (40°C)	64.334 (104°F)
Milk, homogenized			1,548	5,080			
Morpholine	C ₄ H ₉ NO	1.00	1,442	4,731	3.8		
Naphtha		0.76	1,225	4,019			
Natural Gas (37)		0.316 (-103°C)	753 (-103°C)	2,470.5 (-153°F)			
Neon (45)	Ne	1.207 (-246°C)	595 (-246°C)	1,952.1 (-411°F)			
Nitrobenzene (46)	C ₆ H ₅ NO ₂	1.204 (20°C)	1,415 (20°C)	4,642.4 (68°F)		1.514	16.29
Nitrogen (45)	N ₂	0.808 (-199°C)	962 (-199°C)	3,156.2 (-326°F)		0.217 (-199°C)	2.334 (-326°F)
Nitromethane (43)	CH ₃ NO ₂	1.135	1,300	4,265.1	4.0	0.549	5.907
Nonane (23)	C ₉ H ₂ O	0.718 (20°C)	1,207	3,960	4.04	0.99 (20°C)	10.652 (68°F)
1-Nonene (27)	C ₉ H ₁₈	0.736 (20°C)	1,207	3,960	4.0		
Octane (23)	C ₈ H ₁₈	0.703	1,172	3,845.1	4.14	0.73	7.857
n-Octane (29)	C ₈ H ₁₈	0.704 (20°C)	1,212.5	3,978	3.50	0.737	.930)
1-Octene (27)	C ₈ H _{1€}	0.723 (20°C)	1,175.5	3,856.6	4.10		
Oil of Camphor Sassafrassy			1,390	4,560.4	3.8		

Table 2: Sound Speeds in Fluids (cont.)

		given at 2	5°C (77°F) unless	otherwise	noted.	
Substance	Chemical	Specific	Sound	Speed	∆v/°C		matic ty x10 ⁻⁶
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s
Oil, Car (SAE 20a.30)		1.74	870	2,854.3		190	2,045.093
Oil, Castor	C ₁₁ H ₁₀ O ₁₀	0.969	1,477	4,845.8	3.6	0.670	7.209
Oil, Diesel		0.80	1,250	4,101			
Oil, Fuel AA gravity		0.99	1,485	4,872	3.7		
Oil (Lubricating X200)			1,530	5,019.9			
Oil (Olive)		0.912	1,431	4,694.9	2.75	100	1,076.365
Oil (Peanut)		0.936	1,458	4,783.5			
Oil (Sperm)		0.88	1,440	4,724.4			
Oil, 6			1,509 (22°C)	4,951 (72°F)			
2,2-Oxydiethanol	C ₄ H ₁₀ O ₃	1.116	1,586	5,203.4	2.4		
Oxygen (45)	O ₂	1.155 (-186°C)	952 (-186°C)	3,123.4 (-303°F)		0.173	1.861
Pentachloro-ethane (47)	C ₂ HCl ₅	1.687	1,082	3,549.9			
Pentalin (47)	C ₂ HCl ₅	1.687	1,082	3,549.9			
Pentane (36)	C ₅ H ₁₂	0.626 (20°C)	1,020	3,346.5		0.363	3.905
n-Pentane (47)	C ₅ H ₁₂	0.557	1,006	3,300.5		0.41	4.413
Perchlorocyclopentadiene (47)	C₅Cl ₆	1.718	1,150	3,773			
Perchloro-ethylene (47)	C ₂ Cl ₄	1.632	1,036	3,399			
Perfluoro-1-Hepten (47)	C ₇ F ₁₄	1.67	583	1,912.7			
Perfluoro-n-Hexane (47)	C ₆ F ₁₄	1.672	508	1,666.7			
Phene (29, 40, 41)	C ₆ H ₆	0.879	1,306	4,284.8	4.65	0.711	7.65
b-Phenyl acrolein	C ₉ H ₈ O	1.112	1,554	5,098.4	3.2		
Phenylamine (41)	C ₆ H ₅ NO ₂	1.022	1,639	5,377.3	4.0	3.63	39.058
Phenyl bromide (46)	C ₆ H ₅ Br	1.522	1,170 (20°C)	3,838.6 (68°F)		0.693	7.456
Phenyl chloride	C ₆ H ₅ CI	1.106	1,273	4,176.5	3.6	0.722	7.768
Phenyl iodide (46)	C ₆ H ₅ I	1.823	1,114 (20°C)	3,654.9 (68°F)		0.954 (15°C)	10.265 (59°F)

Table 2: Sound Speeds in Fluids (cont.)

		All data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	Δ v /°C		matic ty x10 ⁻⁶
	Formula	Formula Gravity m/s		ft/s	m/s/°C	m²/s	ft ² /s
Phenyl methane (16, 52)	C ₇ H ₈	0.867 (20°C)	1,328 (20°C)	4,357 (68°F)	4.27	0.644	6.929
3-Phenyl propenal	C ₉ H ₈ O	1.112	1,554	5,098.4	3.2		
Phthalardione	C ₈ H ₄ O ₃		1,125 (152°C)	3,691 (306°F)			
Phthalic acid, anhydride	C ₈ H ₄ O ₃		1,125 (152°C)	3,691 (306°F)			
Pthalic anhydride	C ₈ H ₄ O ₃		1,125 (152°C)	3,691 (306°F)			
Pimelic ketone	C ₆ H ₁₀ O	0.948	1,423	4,668.6	4.0		
Plexiglas, Lucite, Acrylic			2,651	8,698			
Polyterpene Resin		0.77	1,099.8 (190°C)	3,608.4 (374°F)		39,000	419,500
Potassium bromide (42)	KBr		1,169 (900°C)	3,835.3 (1652°F)	0.71	.715cp (900°C)	7.693 (1652°F)
Potassium fluoride (42)	KF		1,792 (900°C)	5,879.3 (1652°F)	1.03		
Potassium iodide (42)	кі		985 (900°C)	3,231.6 (1652°F)	0.64		
Potassium nitrate (48)	KNO ₃	1.859 (352°C)	1,740.1 (352°C)	5,709 (666°F)	1.1	1.19 (327°C)	12.804 (621°F)
Propane (2, 13) (-45° to -130°C)	C₃H ₈	0.585 (-45°C)	1,003 (-45°C)	3,290.6 (-49°F)	5.7		
1,2,3-Propanetriol	C ₃ H ₈ O ₃	1.26	1,904	6,246.7	2.2	.000757	
1-Propanol (46)	C ₃ H ₈ O	0.78 (20°C)	1,222 (20°C)	4,009.2 (68°F)			
2-Propanol (46)	C ₃ H ₈ O	0.785 (20°C)	1,170 (20°C)	3,838.6 (68°F)		2.718	29.245
2-Propanone	C ₃ H ₆ O	0.791	1,174	3,851.7	4.5	0.399	4.293
Propene (17, 18, 35)	C₃H ₆	0.563 (-13°C)	963 (-13°C)	3,159.4 (9°F)	6.32		
n-Propyl acetate (22)	C ₅ H ₁₀ O ₂		1,280 (2°C)	4,199 (36°F)	4.63		
n-Propyl-alcohol	C ₃ H ₈ O	0.78 (20°C)	1,222 (20°C)	4,009.2 (68°F)		2.549	27.427
Propylchloride (47)	C ₃ H ₇ CI	0.892	1,058	3,471.1		0.378	4.067

Table 2: Sound Speeds in Fluids (cont.)

		Ali data	given at 2	5°C (77°F) unless	otherwise	noted.
Substance	Chemical	Specific	Sound	Speed	Δ v /°C		matic ty x10 ⁻⁶
	Formula	Gravity	m/s ft/s		m/s/°C	m²/s	ft ² /s
Propylene (17, 18, 35)	C₃H ₆	0.563 (-13°C)	963 (-13°C)	(3159.4) (9°F)	6.32		
Pyridine	C ₆ H ₅ N	0.982	1,415	4,642.4	4.1	0.992 (20°C)	10.673 (68°F)
Refrigerant 11 (3, 4)	CCl₃F	1.49	828.3 (0°C)	2,717.5 (32°F)	3.56		
Refrigerant 12 (3)	CCI ₂ F ₂	1.516 (-40°C)	774.1 (-40°C)	2,539.7 (-40°F)	4.24		
Refrigerant 14 (14)	CF ₄	1.75 (-150°C)	875.24 (-150°C)	2,871.5 (-238°F)	6.61		
Refrigerant 21 (3)	CHCl₂F	1.426 (0°C)	891 (0°C)	2,923.2 (32°F)	3.97		
Refrigerant 22 (3)	CHCIF ₂	1.491 (-69°C)	893.9 (50°C)	2,932.7 (122°F)	4.79		
Refrigerant 113 (3)	CCI ₂ F-CCIF ₂	1.563	783.7 (0°C)	2,571.2 (32°F)	3.44		
Refrigerant 114 (3)	CCIF ₂ -CCIF ₂	1.455	665.3 (-10°C)	2,182.7 (14°F)	3.73		
Refrigerant 115 (3)	C ₂ CIF ₅		656.4 (-50°C)	2,153.5 (-58°F)	4.42		
Refrigerant C318 (3)	C ₄ F ₈	1.62 (-20°C)	574 (-10°C)	1,883.2 (14°F)	3.88		
Selerium (8)	Se		1,072 (250°C)	3,517.1 (482°F)	0.68		
Silicone (30 cp)		0.993	990	3,248		30	322.8
Sodium fluoride (42)	NaF	0.877	2,082 (1000°C)	6,830.7 (1832°F)	1.32		
Sodium nitrate (48)	NaNO ₃	1.884 (336°C)	1,763.3 (336°C)	5,785.1 (637°F)	0.74	1.37 (336°C)	14.74 (637°F)
Sodium nitrite (48)	NaNO ₂	1.805 (292°C)	1,876.8 (292°C)	6,157.5 (558°F)			
Solvesso #3		0.877	1,370	4,494.8	3.7		
Spirit of wine	C ₂ H ₆ O	0.789	1,207	3,960	4.0	1.396	15.02
Sulfur (7, 8, 10)	s		1,177 (250°C)	3,861.5 (482°F)	-1.13		
Sulfuric Acid (1)	H ₂ SO ₄	1.841	1,257.6	4,126	1.43	11.16	120.081

Table 2: Sound Speeds in Fluids (cont.)

		All data given at 25°C (77°F) unless otherwise noted.								
Substance	Chemical	Specific	Sound	Speed	∆v/°C		matic ty x10 ⁻⁶			
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s			
Tellurium (7)	Te		991 (450°C)	3,251.3 (842°F)	0.73					
1,1,2,2-Tetrabromo-ethane (47)	C ₂ H ₂ Br ₄	2.966	1,027	3,369.4						
1,1,2,2-Tetrachloro-ethane (67)	C₂H₂Cl₄	1.595	1,147	3,763.1		1.156 (15°C)	12.438 (59°F)			
Tetrachloroethane (46)	C₂H₂Cl₄	1.553 (20°C)	1,170 (20°C)	3,838.6 (68°F)		1.19	12.804			
Tetrachloro-ethene (47)	C ₂ Cl ₄	1.632	1,036	3,399						
Tetrachloro-Methane (33, 47)	CCI ₄	1.595 (20°C)	926	3,038.1		0.607	6.531			
Tetradecane (46)	C ₁₄ H ₃ O	0.763 (20°C)	1,331 (20°C)	4,366.8 (68°F)		2.86 (20°C)	30.773 (68°F)			
Tetraethylene glycol	C ₈ H ₁₈ O ₅	1.123	1,586	5,203.4	3.0					
Tetrafluoro-methane (14) (Freon 14)	CF ₄	1.75 (-150°C)	875.24 (-150°C)	2,871.5 (-238°F)	6.61					
Tetrahydro-1,4-isoxazine	C ₄ H ₉ NO	1.000	1,442	4,731	3.8					
Toluene (16, 52)	C ₇ H ₈	0.867 (20°C)	1,328 (20°C)	4,357 (68°F)	4.27	0.644	6.929			
o-Toluidine (46)	C ₇ H ₉ N	0.999 (20°C)	1,618	5,308.4		4.394 (20°C)	47.279 (68°F)			
p-Toluidine (46)	C ₇ HgN	0.966 (45°C)	1,480	4,855.6		1.863 (50°C)	20.053 (122°F)			
Toluol	C ₇ H ₈	0.866	1,308	4,291.3	4.2	0.58	6.24			
Tribromo-methane (46, 47)	CHBr ₃	2.89 (20°C)	918	3,011.8		0.654	7.037			
1,1,1-Trichloro-ethane (47)	C ₂ H ₃ Cl ₃	1.33	985	3,231.6		0.902 (20°C)	9.705 (68°F)			
Trichloro-ethene (47)	C ₂ HCl ₃	1.464	1,028	3,372.7						
Trichloro-fluoromethane (3) (Freon 11)	CCl₃F	1.49	828.3 (0°C)	2,717.5 (32°F)	3.56					
Trichloro-methane (47)	CHCl ₃	1.489	979	3,211.9	3.4	0.55	5.918			
1,1,2-Trichloro- 1,2,2-Trifluoro-Etham	CCI ₂ F-CCIF ₂	1.563	783.7 (0°C)	2,571.2 (32°F)						
Triethyl-amine (33)	C ₆ H ₁₅ N	0.726	1,123	3,684.4	4.47					

Table 2: Sound Speeds in Fluids (cont.)

		All data given at 25°C (77°F) unless otherwise noted.							
Substance	Chemical	Specific Gravity	Sound	Speed	∆v/°C		matic ty x10 ⁻⁶		
	Formula	Gravity	m/s	ft/s	m/s/°C	m²/s	ft ² /s		
Triethylene glycol	C ₆ H ₁₄ O ₄	1.123	1,608	5,275.6	3.8				
1,1,1-Trifluoro- 2-Chloro-2-Bromo-Ethane	C ₂ HClBrF ₃	1.869	693	2,273.6					
1,2,2-Trifluorotrichloro- ethane (Freon 113)	CCI ₂ F-CCIF ₂	1.563	783.7 (0°C)	2,571.2 (32°F)	3.44				
d-1,3,3-Trimethylnorcamphor	C ₁₀ H ₁₆ O	0.947	1,320	4,330.7		0.22	2.367		
Trinitrotoluene (43)	C ₇ H ₅ (NO ₂) ₃	1.64	1,610 (81°C)	5,282.2 (178°F)					
Turpentine		0.88	1,255	4,117.5		1.4	15.064		
Unisis 800		0.87	1,346	4,416					
Water, distilled (49, 50)	H ₂ O	0.996	1,498	4,914.7	-2.4	1.00	10.76		
Water, heavy	D ² O		1,400	4,593					
Water, sea		1.025	1,531	5,023	-2.4	1.00	10.76		
Wood Alcohol (40, 41)	CH ₄ O	0.791 (20°C)	1,076	3,530.2	2.92	0.695	7.478		
Xenon (45)	Xe		630 (-109°C)	2,067 (-164°F)					
m-Xylene (46)	C ₈ H ₁₀	0.868 (15°C)	1,343 (20°C)	4,406.2 (68°F)		0.749 (15°C)	8.059 (59°F)		
o-Xylene (29, 46)	C ₈ H ₁₀	0.897 (20°C)	1,331.5	4,368.4	4.1	0.903 (20°C)	9.716 (68°F)		
p-Xylene (46)	C ₈ H ₁₀		1,334 (20°C)	4,376.6 (68°F)		0.662	7.123		
Xylene hexafluoride	C ₈ H ₄ F ₆	1.37	879	2,883.9		0.613	6.595		
Zinc (7)	Zn		3,298 (450°C)	10,820.2 (842°F)					

6.3 SOUND SPEEDS IN WATER AT SELECTED TEMPERATURES

Table 3: Sound Speeds in Water at Selected Temperatures

Temp	erature	Sound Spe	ed in Water	Temp	erature	Sound Spe	ed in Water
°C	°F	m/s	ft/s	°C	°F	m/s	ft/s
0	32.0	1,402	4,600				
1	33.8	1,407	4,616	31	87.8	1,511	4,958
2	35.6	1,412	4,633	32	89.6	1,513	4,964
3	37.4	1,417	4,649	33	91.4	1,515	4,971
4	39.2	1,421	4,662	34	93.2	1,517	4,977
5	41.0	1,426	4,679	35	95.0	1,519	4,984
6	42.8	1,430	4,692	36	96.8	1,521	4,990
7	44.6	1,434	4,705	37	98.6	1,523	4,997
8	46.4	1,439	4,721	38	100.4	1,525	5,004
9	48.2	1,443	4,734	39	102.2	1,527	5,010
10	50.0	1,447	4,748	40	104.0	1,528	5,013
11	51.8	1,451	4,761	41	105.8	1,530	5,020
12	53.6	1,455	4,774	42	107.6	1,532	5,026
13	55.4	1,458	4,784	43	109.4	1,534	5,033
14	57.2	1,462	4,797	44	111.2	1,535	5,036
15	59.0	1,465	4,807	45	113.0	1,536	5,040
16	60.8	1,469	4,820	46	114.8	1,538	5,046
17	62.6	1,472	4,830	47	116.6	1,539	5,049
18	64.4	1,476	4,843	48	118.4	1,540	5,053
19	66.2	1,479	4,853	49	120.2	1,541	5,056
20	68.0	1,482	4,862	50	122.0	1,543	5,063
21	69.8	1,485	4,872	51	123.8	1,543	5,063
22	71.6	1,488	4,882	52	125.6	1,544	5,066
23	73.4	1,491	4,892	53	127.4	1,545	5,069
24	75.2	1,493	4,899	54	129.2	1,546	5,072
25	77.0	1,496	4,908	55	131.0	1,547	5,076
26	78.8	1,499	4,918	56	132.8	1,548	5,079
27	80.6	1,501	4,925	57	134.6	1,548	5,079
28	82.4	1,504	4,935	58	136.4	1,549	5,082
29	84.2	1,506	4,941	59	138.2	1,550	5,086
30	86.0	1,509	4,951	60	140.0	1,550	5,086

Table 3: Sound Speeds in Water at Selected Temperatures (cont.)

Temp	erature	Sound Spe	ed in Water	Temp	erature	Sound Spe	ed in Water
°C	°F	m/s	ft/s	°C	°F	m/s	ft/s
61	141.8	1,551	5,089	96	204.8	1,546	5,072
62	143.6	1,552	5,092	97	206.6	1,545	5,069
63	145.4	1,552	5,092	98	208.4	1,544	5,066
64	147.2	1,553	5,095	99	210.2	1,543	5,063
65	149.0	1,553	5,095	100	212.0	1,543	5,063
66	150.8	1,553	5,095	104	220.0	1,538	5,046
67	152.6	1,554	5,099	110	230.0	1,532	5,026
68	154.4	1,554	5,099	116	240.0	1,524	5,000
69	156.2	1,554	5,099	121	250.0	1,526	5,007
70	158.0	1,554	5,099	127	260.0	1,507	4,944
71	159.8	1,554	5,099	132	270.0	1,497	4,912
72	161.6	1,555	5,102	138	280.0	1,487	4,879
73	163.4	1,555	5,102	143	290.0	1,476	4,843
74	165.2	1,555	5,102	149	300.0	1,465	4,807
75	167.0	1,555	5,102	154	310.0	1,453	4,767
76	168.8	1,555	5,102	160	320.0	1,440	4,725
77	170.6	1,554	5,099	166	330.0	1,426	4,679
78	172.4	1,554	5,099	171	340.0	1,412	4,633
79	174.2	1,554	5,099	177	350.0	1,398	4,587
80	176.0	1,554	5,099	182	360.0	1,383	4,538
81	177.8	1,554	5,099	188	370.0	1,368	4,488
82	179.6	1,553	5,095	193	380.0	1,353	4,439
83	181.4	1,553	5,095	199	390.0	1,337	4,387
84	183.2	1,553	5,095	204	400.0	1,320	4,331
85	185.0	1,552	5,092	210	410.0	1,302	4,272
86	186.8	1,552	5,092	216	420.0	1,283	4,210
87	188.6	1,552	5,092	221	430.0	1,264	4,147
88	190.4	1,551	5,089	227	440.0	1,244	4,082
89	192.2	1,551	5,089	232	450.0	1,220	4,003
90	194.0	1,550	5,086	238	460.0	1,200	3,937
91	195.8	1,549	5,082	243	470.0	1,180	3,872
92	197.6	1,549	5,082	249	480.0	1,160	3,806
93	199.4	1,548	5,079	254	490.0	1,140	3,740
94	201.2	1,547	5,076	260	500.0	1,110	3,642
95	203.0	1,547	5,076				

6.4 PIPE SIZE DATA

Table 4: Standard ANSI Data for Carbon Steel and Stainless Steel Pipe

			Α	В	С	Г				Α	В	С				
Nominal	Outside	Wall	Carbon	Carbon	Stainless		Nominal	Outside	Wall	Carbon	Carbon	Stainless Steel				
Pipe		Thickness		Steel	Steel	ı	Pipe		Thickness		Steel					
Size (in.)	(In.)	(in.)	Wall Thickness	Schedule Number	Number	ı	Stze (In.)	(In.)	(in.)	Wall Thickness	Schedule Number	Schedule Number				
(111.)			Desig.		Number	ı	(11.7			Desig.		realition				
		0.049	-	-	10S				0.065	-	-	5S				
1/8	0.405	0.068	STD	40	40S		I		0.109	-	-	108				
$ldsymbol{le}}}}}}$		0.095	XS	80	80S	ı	2	0.075	0.154	STD	40	40S				
I		0.065	-	-	10S	ļ		2.375	0.218	XS	80	80S				
1/4	0.540	0.088	STD	40	40S				0.344	-	160	-				
ldot		0.119	XS	80	80S	ı	ldot	\vdash	0.436	XXS	-	-				
		0.065	-	-	108				0.083	-	-	58				
3/8	0.675	0.091	STD	40	40S		I		0.120	-	-	108				
ldot		0.126	XS	80	80S	ı	2 1/2	2.875	0.203	STD	40	40S				
I		0.065	-	-	58		2 1/2	2.010	0.276	XS	80	80S				
I		0.083	-	-	108		I		0.375	-	160	-				
1/2	0.840	0.109	STD	40	408		ldot		0.552	XXS	-	-				
1/2	0.640	0.147	XS	80	80S		I		0.083	-	-	58				
I		0.187	-	160	-		I		0.120	-	-	108				
\vdash		0.294	XXS	-	-	ı	3	3.500	0.216	STD	40	40S				
I		0.065	-	-	58		,		0.300	XS	80	80S				
I		0.083	-	-	108		I		0.438	-	160	-				
3/4	1.050	0.113	STD	40	40S				0.600	XXS	-	-				
5/4	1.000	0.154	XS	80	80S		I		0.083	-	-	58				
I		0.218		160	-	3 1/2	3 1/2	2.15	Н	ļ	2 1 12	4.000	0.120	- OTD	- 40	10S
\vdash		0.308	XXS	-	- 58			3 1/2	4.000	0.226	STD	40	40S			
I		0.065	-	-					0.318	XS	80	80S				
I		0.109	- OTD	- 40	108		\vdash		0.636	XXS		-				
1	1.315	0.133	STD	40	408		I		0.083	-	-	58				
I ' I	1.515	0.179	XS	80	80S		I		0.120	- OTD	- 40	10S				
I		0.250	-	160	-		I	4.500	0.237	STD	40	40S				
\vdash		0.358	XXS	-	- 5S	ı	4	4.555	0.337	XS	80	80S				
I		0.065	-	-	108		I		0.438 0.531	-	120 160	-				
I		0.140	STD	40	408		I		0.674	vve		-				
1 1/4	1.660	0.140	XS	80	80S		\vdash		0.109	XXS	-	- 5S				
		0.191		160			I		0.134	-	-	10S				
I			- vve		-		I			- etd	40					
$\vdash \vdash$	—	0.382	XXS	-	- 5S	<u> </u>	5.536	0.258	STD	40 80	40S 80S					
		0.109	-	-	108			0.500		120						
		0.109	STD	40	408			0.625	-	160	-					
1 1/2	1.900	0.145	XS	80	80S			0.750	XXS		-					
' '-		0.281		160			$\vdash \vdash$	\vdash	0.750	^^>	-	-				
		0.400	XXS	- 160	-		\vdash									
		0.400	7/10	_	_	_										

Table 4: Standard ANSI Data for Carbon Steel and Stainless Steel Pipe (cont.)

			Α	В	С					Α	В	С																
Nominal	Outside	Wall	Carbon	Carbon	Stainless	П	Nominal	Outside	Wall	Carbon	Carbon	Stainless																
Pipe		Thickness	Steel	Steel	Steel	П	Pipe		Thickness		Steel	Steel																
Stze (In.)	(In.)	(in.)	Wall Thickness	Schedule Number	Schedule Number	П	Stze (In.)	(ln.)	(in.)	Wall Thickness	Schedule Number	Schedule Number																
(iii)			Desig.	.,		П	(11.7			Desig.	.40																	
		0.109	-	-	58	П			0.156		-	58																
I		0.134	-	-	108	П			0.188	-	-	10S																
1	6.625	0.280	STD	40	40S	П	1		0.250	-	10	-																
6	0.025	0.432	XS	80	80S	П			0.312	-	20	-																
1		0.562 0.719	-	120 160	-	П			0.375 0.438	STD	30 40	-																
1		0.864	xxs	160	-	П			0.438	XS	40	-																
$\vdash \vdash$		0.109	-	-	58	П	14	14.000	0.594		60	-																
1		0.148	-	-	108	П	14		0.625	XXS	-	-																
1		0.250	-	20	-	П			0.750	-	80	-																
		0.277	-	30	-	H			0.938	-	100	-																
1		0.322	STD	40	40S	il			1.094	-	120	-																
1	8.625	0.406	-	60	-	ı			1.250	-	140	-																
8	8.625	0.500	XS	80	80S	П			1.406	-	160	-																
1		0.594	-	100	-	П			0.165	-	-	58																
1		0.719	-	120	-	l			0.188	-	-	108																
1		0.812	-	140	-	П			0.250	-	10	-																
1		0.875	XXS	-	-	П			0.312	-	20	-																
\vdash		0.906	-	160	-	П			0.375	STD	30	-																
1		0.134 0.165	-	-	5S 10S	Н	16	16.000	0.500	XS	40 60	-																
1		0.165	-	20		i '°	! '°	! '°	! '°	i '°	16	16	16		0.656 0.844	-	80	-										
1		0.307	-	30	-						 	i I	11	1						1.031	-	100	-					
1		0.365	STD	40	40S	П	1 1		1.219	-	120	-																
10	10.750	0.500	XS	60	808	П			1.439	-	140	-																
		0.594	-	80	-	ı			1.594	-	160	-																
1		0.719	-	100	-	i			0.165	-	-	58																
1		0.844	-	120	-	П			0.188	-	-	108																
		1.000	XXS	140	-	П			0.250	-	10	-																
		0.156	-	-	58	П			0.312	-	20	-																
I		0.180	-	-	108	П			0.375	STD	-	-																
1		0.250	-	20	-	П			0.438	-	30	-																
I		0.330	- etb	30	400	П	4.0	18.000	0.500	XS	- 40	-																
		0.375 0.406	STD -	40	40S	П	18		0.562		40 60	-																
1	12.750	0.406	XS	40	80S	Н			0.750 0.938	-	80																	
12		0.562	- ^3	60	600	П			1.156	-	100	-																
		0.688	-	80	-					1.375	-	120	-															
		0.844		100	-		-{	-{	-{	{		{	-{												1.562	-	140	-
		1.000	xxs	120	-				1.781	-	160	-																
		1.125	-	140	-	H																						
		1.312	-	160	-																							

Table 4: Standard ANSI Data for Carbon Steel and Stainless Steel Pipe (cont.)

			Α	В	С	Г				Α	В	С
Nominal	Outside	Wall	Carbon	Carbon	Stainless		Nominal	Outside	Wall	Carbon	Carbon	Stainless
Pipe	Diameter	Thickness	Steel	Steel	Steel		Pipe		Thickness		Steel	Steel
Stze	(In.)	(In.)		Schedule			Stze	(In.)	(In.)	Wall	Schedule	
(in.)			Thickness Desig.	Number	Number		(ln.)			Thickness Desig.	Number	Number
-		0.188	-	-	5S		\vdash		0.250	-	-	5S
I		0.218	-	-	108	i	I		0.312	-	10	108
I		0.250	-	10	-	i	I I		0.375	STD	-	-
I		0.375	STD	20	-	ı	30	30.000	0.500	XS	20	-
I		0.500	XS	30	-	i			0.625	-	30	-
I		0.594	-	40	-	i			0.750	-	40	-
20	20.000	0.812	-	60	-	i			0.312	-	10	-
		1.031	-	80	-	i		İ	0.375	STD	-	-
I		1.281	-	100	-	i	32	32.000	0.500	XS	20	-
I		1.500	-	120	-	i	32		0.625	-	30	-
		1.750	-	140	-	i			0.688	-	40	-
		1.969	-	160	-	i	$\vdash \vdash$		0.344	-	10	-
		0.188	-	-	5S		I		0.375	STD	-	-
I		0.218	-	-	10S	i	34	34.000	0.500	XS	20	-
I		0.250	-	10	-	i			0.625	-	30	-
I		0.375	STD	20	-	i	I I		0.688	-	40	-
I		0.500	XS	30	-	i			0.312	-	10	-
22	22.000	0.875	-	60	-	i	I		0.375	STD	-	-
22		1.125	-	80	-	i	36	36.000	0.500	XS	20	-
I		1.375	-	100	-	i	55		0.625	-	30	-
I		1.625	-	120	-	i	I		0.750	-	40	-
I		1.875	-	140	-	i			0.375	STD	-	-
I		2.125	-	160	-	ı	l l		0.500	XS	20	-
		0.218	-	-	5S		42	42.000	0.625	-	30	-
I		0.250	-	10	10S	ı			0.750	-	40	-
I		0.375	STD	20	-	ı	48		0.375	STD	-	-
I		0.500	XS	-	-	ı	40	48.000	0.500	XS	-	-
I		0.562	-	30	-	ı						
I	24.000	0.688	-	40	-	ı						
24	24.000	0.969	-	60	-	ı						
I		1.219	-	80	-	ı						
I		1.531	-	100	-	ı						
I		1.812	-	120	-							
		2.062	-	140	-							
		2.344	-	160	-							
		0.312	-	10	-							
26	26.000	0.375	STD	-	-							
		0.500	XS	20	-							
		0.312	-	10	-							
28	00.000	0.375	STD	-	-							
26	28.000	0.500	XS	20	-							
		0.625	-	30	-							

Table 5: Cast Iron Pipe Data - Standard Classes

	Clas	ss A	Clas	ss B	Clas	ss C	Clas	ss D
Nominal	Outside	Wall	Outside	Wall	Outside	Wall	Outside	Wall
Pipe Size	Diameter	Thickness	Diameter	Thickness	Diameter	Thickness	Diameter	Thickness
(In.)	(In.)	(In.)	(In.)	(In.)	(In.)	(in.)	(In.)	(in.)
3	3.80	0.39	3.96	0.42	3.96	0.45	3.96 5.00	0.48
4	4.80	0.42	5.00	0.45	5.00	0.40		0.52
6	6.90	0.44	7.10	0.48	7.10	0.51	7.10	0.55
8	9.05	0.46	9.05	0.51	9.30	0.56	9.30	0.60
10	11.10	0.50	11.10	0.57	11.40	0.62	11.40	0.68
12	13.20	0.54	13.20	0.62	13.50	0.68	13.50	0.75
14	15.30	0.57	15.30	0.66	15.65	0.74	15.65	0.82
16	7.40	0.60	17.40	0.70	17.80	0.80	17.80	0.89
18	19.50	0.64	19.50	0.75	19.92	0.87	19.92	0.96
20	21.60	0.67	21.60	0.80	22.06	0.92	22.06	1.03
24	25.80	0.76	25.80	0.89	26.32	1.05	26.32	1.16
30	31.74	0.88	32.00	1.03	32.40	1.20	32.74	1.37
32	37.96	0.99	38.30	1.15	38.70	1.36	39.16	1.58
42	44.20	1.10	44.50	1.28	45.10	1.54	45.58	1.78
48	50.50	1.26	50.80	1.42	51.40	1.71	51.98	1.99
54	56.66	1.35	57.10	1.55	57.80	1.90	58.40	2.23
60	62.80	1.39	63.40	1.67	64.20	2.00	64.82	2.38
72	75.34	1.62	76.00	1.95	76.88	2.39		
	07.54	4.70	88.54	2.22				
84	87.54	1.72	00.04	2.22				
84								
	Clas	ss E	Cla	ss F		ss G		ss H
Nominal	Cla: Outside	ss E Wall	Cla Outside	ss F Wall	Outside	Wall	Outside	Wall
Nominal Pipe Size	Clas Outside Diameter	ss E Wall Thickness	Cla Outside Diameter	ss F Wall Thickness	Outside Diameter	Wall Thickness	Outside Diameter	Wall Thickness
Nominal Pipe Size (In.)	Cla: Outside	ss E Wall	Cla Outside	ss F Wall	Outside	Wall	Outside	Wall
Nominal Pipe Size (In.) 3	Clas Outside Diameter	ss E Wall Thickness	Cla Outside Diameter	ss F Wall Thickness	Outside Diameter	Wall Thickness	Outside Diameter	Wall Thickness
Nominal Pipe Size (In.) 3	Clas Outside Diameter (in.)	ss E Wall Thickness (In.)	Cla Outside Diameter (In.)	ss F Wall Thickness (in.)	Outside Diameter (In.)	Wali Thickness (In.)	Outside Diameter (In.)	Wall Thickness (In.)
Nominal Pipe Size (In.) 3 4	Clas Outside Diameter (In.)	ss E Wall Thickness (In.)	Cla Outside Diameter (In.) 7.22	ss F Wall Thickness (In.)	Outside Diameter (In.) 7.38	Wall Thickness (In.)	Outside Diameter (In.) 7.38	Wall Thickness (in.)
Nominal Pipe Size (In.) 3 4 6	Clas Outside Diameter (in.) 7.22 9.42	ss E Wall Thickness (In.) 0.58	Cla Outside Diameter (in.) 7.22 9.42	ss F Wall Thickness (In.) 0.61 0.66	Outside Diameter (In.) 7.38 9.60	Wall Thickness (In.) 0.65 0.75	Outside Diameter (In.) 7.38 9.60	Wall Thickness (in.) 0.69 0.80
Nominal Pipe Size (in.) 3 4 6 8	Clas Outside Diameter (in.) 7.22 9.42 11.60	Wall Thickness (In.) 0.58 0.66 0.74	Cla Outside Diameter (In.) 7.22 9.42 11.60	ss F Wall Thickness (in.) 0.61 0.66 0.80	Outside Diameter (In.) 7.38 9.60 11.84	Wall Thickness (In.) 0.65 0.75 0.86	Outside Diameter (In.) 7.38 9.60 11.84	Wall Thickness (In.) 0.69 0.80 0.92
Nominal Pipe Size (In.) 3 4 6 8 10	Classide Diameter (In.) 7.22 9.42 11.60 13.78	Wall Thickness (In.) 0.58 0.66 0.74 0.82	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78	SS F Wall Thickness (In.) 0.61 0.66 0.80 0.89	Outside Diameter (In.) 7.38 9.60 11.84 14.08	Wall Thickness (in.) 0.65 0.75 0.86 0.97	Outside Diameter (In.) 7.38 9.60 11.84 14.08	Wall Thickness (In.) 0.69 0.80 0.92 1.04
Nominal Pipe Size (In.) 3 4 6 8 10 12	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98	ss E Wall Thickness (in.) 0.58 0.66 0.74 0.82 0.90	Cla Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98	SS F Wall Thickness (in.) 0.61 0.66 0.80 0.89 0.99	7.38 9.60 11.84 14.08	Wall Thickness (In.) 0.65 0.75 0.86 0.97 1.07	Outside Diameter (In.) 7.38 9.60 11.84 14.08 16.32	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16
Nominal Pipe Size (in.) 3 4 6 8 10 12 14	Clas Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16	988 E Wall Thickness (In.) 0.58 0.66 0.74 0.82 0.90	Cla Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99	7.38 9.60 11.84 14.08 16.32 18.54	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07	7.38 9.60 11.84 14.08 16.32 18.54	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34	988 E Wall Thickness (In.) 0.58 0.66 0.74 0.82 0.90 0.90	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34	SS F Wall Thickness (in.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17	7.38 9.60 11.84 14.08 16.32 18.54 20.78	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28	7.38 9.60 11.84 14.08 16.32 18.54 20.78	Wall Thickness (In.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54	Wall Thickness (in.) 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15	Cla Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54	SS F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (in.) 3 4 6 8 10 12 14 16 18 20 24	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90	988 E Wall Thickness (In.) 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31	Cla Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90	SS F Wall Thickness (in.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45	7.38 9.60 11.84 14.08 16.32 18.54 20.78	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28	7.38 9.60 11.84 14.08 16.32 18.54 20.78	Wall Thickness (In.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18 20 24 30	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.10	9.58 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31 1.55	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.46	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45 1.73	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18 20 24 30 32	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90	988 E Wall Thickness (In.) 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31	Cla Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90	SS F Wall Thickness (in.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18 20 24 30 32 42	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.10	9.58 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31 1.55	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.46	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45 1.73	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (in.) 3 4 6 8 10 12 14 16 18 20 24 30 32 42 48	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.10	9.58 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31 1.55	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.46	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45 1.73	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18 20 24 30 32 42 48 54	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.10	9.58 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31 1.55	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.46	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45 1.73	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18 20 24 30 32 42 48 54 60	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.10	9.58 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31 1.55	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.46	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45 1.73	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39 1.51
Nominal Pipe Size (In.) 3 4 6 8 10 12 14 16 18 20 24 30 32 42 48 54	Clas Outside Diameter (in.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.10	9.58 0.58 0.66 0.74 0.82 0.90 0.90 1.07 1.15 1.31 1.55	Cla Outside Diameter (In.) 7.22 9.42 11.60 13.78 15.98 18.16 20.34 22.54 26.90 33.46	ss F Wall Thickness (In.) 0.61 0.66 0.80 0.89 0.99 1.08 1.17 1.27 1.45 1.73	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.65 0.75 0.86 0.97 1.07 1.18 1.28 1.39	7.38 9.60 11.84 14.08 16.32 18.54 20.78 23.02	Wall Thickness (in.) 0.69 0.80 0.92 1.04 1.16 1.27 1.39

Table 6: Ductile Iron Pipe Data - Standard Classes

Nominal	Outside			Pipe Wa	all Thickne	ss (in.)		
Pipe Size (in.)	Diameter (in.)	Class 50	Class 51	Class 52	Class 53	Class 54	Class 55	Class 56
3	3.96		0.25	0.28	0.31	0.43	0.37	0.40
4	4.90		0.26	0.29	0.32	0.35	0.38	0.41
6	6.90	0.25	0.28	0.31	0.34	0.37	0.40	0.43
8	9.05	0.27	0.30	0.33	0.36	0.39	0.42	0.45
10	11.10	0.29	0.32	0.35	0.38	0.44	0.47	
12	13.20	0.31	0.34	0.37	0.40	0.43	0.46	0.49
14	15.30	0.33	0.36	0.39	0.42	0.45	0.48	0.51
16	17.40	0.34	0.37	0.40	0.43	0.46	0.49	0.52
18	19.50	0.35	0.38	0.41	0.44	0.47	0.50	0.53
20	21.60	0.36	0.39	0.42	0.45	0.48	0.51	0.54
24	25.80	0.38	0.41	0.44	0.47	0.50	0.53	0.56
30	32.00				0.51	0.55	0.59	0.63
36	38.30				0.58	0.63	0.68	0.73
42	44.50				0.65	0.71	0.77	0.83
48	50.80				0.72	0.79	0.86	0.93
54	57.10				0.81	0.89	0.97	1.05

7 EC- DECLARATION OF CONFORMITY

B.M. TECNOLOGIE INDUSTRIALI

hereby certifies

THAT THE DEVICES THIS MANUAL REFERS TO ARE IN CONFORMITY WITH APPLICABLE EUROPEAN DIRECTIVES:

89/336/EEC-EMC

73/23/EEC- LOW VOLTAGE

APPLIED STANDARDS:

EN50081:1992

BS EN61010-1:1993



Management system as per

EN ISO 9001: 2000

in accordance with TÜV NORD CERT procedures, it is hereby certified that


B.M. Tecnologie Industriali S.r.l.

Via Praimbole, 13 35010 Limena (PD) Italy

applies a management system in line with the above standard for the following scope

Design, assembly and installation of industrial automation systems. Sale, assembly and installation of industrial automation systems.

Gertificate Registration No. 44 100 090284 Audit Report No. 3504 3819 Valid until 2010-11-15



Essen, 2009-05-20

This certification was conducted in accordance with the TÜV NÓRD CERT auditing and certification precedures and is subject to regular surveillance audits.

TOV NORD CERT GMbH

Langemarcksträsse 20

45141 Essen

www.tuev-nord-cert.com



Ultrasonic Transit Time Flow meter TTFM100 Series

Because of B.M. Tecnologie Industriali's policy of improving their products, the TTFM100 series, would be revised and improved.

Please inform us about misunderstandings or errors which you may find in this manual comparing it to the device you bought.

Do not hesitate to contact us to suggest how to improve our devices, thank You.

B.M. TECNOLOGIE INDUSTRIALI s.r.l.

Via Praimbole, 13-35010 LIMENA (PD)-ITALY

Tel. +39(0)49-8841651 - Fax +39(0)49-8841654

e-mail: bm@bmtecnologie.it – web: www.bmtecologie.it



Ultrasonic Transit Time Flow meter TTFM100 SERIES PC Data Logger





It is supposed to have some Personal Computer (PC) knowledge before starting reading this manual.

The information listed below is of general kind. Please be informed that a Laptop PC with Windows[©] XP[©] Operating System.

1. Required Hardware

For information about the serial port and the connection cable, please refer to Chapter 5 of TTFM100 instructions manual.

🖳 Device Manager


Note:

Your PC has normally more than one USB ports so you need a converter for the serial connection to TTFM100 series instrument.

If you use the wall mounted version, you need a RS485 to USB converter.

If you use the portable version, you need a RS232 to USB converter

During the set-up and the data logging, the port number the system gives to the added USB serial converter is required; please

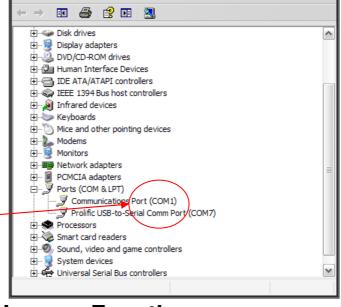

2. Initial settings for Data Logger Function

Please Ref. to Chapter 3.10.1 for a general description of Data Logger function.

In the following example, only a few measure, available on the serial RS485-RS232, are set in ON. The user could set ON other measure.

It is supposed the PC is ready to work. Normally with the operating system, there is a program for perform a serial communications between various device and PC.


In this case we use a direct connection without any modem and the follow example is based on HyperTerminal[©] by Hilgraeve Inc. The last free version included with the Microsoft[©] Windows[©] Operating Systems is the "6.3" and is possible to download it from Internet. The next version "7.xx" will be payment software.

B.M. Tecnologie Industriali Via Praimbole 13 35010 LIMENA (PD) Cod.Fis./P.Iva IT02459940280



Tel. +39 (0) 49 884.16.51 Fax +39 (0) 49 884.16.54 E-Mail bm@bmtecnologie.it Web www.bmtecnologie.it





Pag. 102 di

2.1 TTFM100 - TTFM100B Settings (Wall mount and Portable)

Note:


The portable type TTFM100B does not give information about the analog signals and the calorimeter, but all the other settings are the same.

The TTFM100B display's has a different format but the information shown is the same.

Wall Mounted Version	Portable Version	Press
Data Logger Option ON	M50 Logger Option ON	MENU 5 0
Data Logger Setup[51 Next =xx:xx:xx XXXX	M51 Logger Setup Start **:**:** Interval 00:00:30 Go On **:**:**	MENU 5 1
Data Logger Setup[51 Start Time = **: **: **	M52 Data Direction 1. To Buffer	▼/-)
Data Logger Setup[51 Interval =00:00:30	M53 Buffer Viewer Press ENT to go	▼/-
Data Logger Setup[51 Log Times = 1000		▼/-
Data Logger Setup[51 Next =xx:xx:xx XXXX		








Pag. 103 di 126

The follow table, for example, show the measure set to ON for the instruments, wall mount and portable.

WALL MOUNT	SET	PORTABLE	SET
0. Date and Time	ON	0.	
1. System Status	ON	1. Date and Time	ON
2. Current Window	OFF	2. System Status	ON
3. Signal Strength	ON	3. Current Window	OFF
4. Flow Rate	ON	4. Flow Rate	ON
5. Velocity	ON	5. Velocity	ON
6. NET Totalized	OFF	6. NET Totalized	OFF
7. POS Totalized	ON	7. POS Totalized	ON
8. NEG Totalized	OFF	8. NEG Totalized	OFF
9. Energy Flow Rate	OFF	9. Signal Strength	ON
10. Energy NET Total	OFF	10. Working Timer	OFF
11. Energy POS Total	OFF	11. Flow Today	OFF
12. Energy NEG Total	OFF	Not applicable	
13. Fluid Velocity	OFF	Not applicable	
14. RTD T1	OFF	Not applicable	
15. RTD T2	OFF	Not applicable	
16. Analog Input 3	OFF	Not applicable	
17. Analog Input 4	OFF	Not applicable	
18. Analog Input 5	OFF	Not applicable	
19. Working Timer	OFF	Not applicable	
20. Flow Today	OFF	Not applicable	
21. Serial Number	OFF	Not applicable	









Pag. 104 di

2.2 Hardware connections between TTFM100 & PC

For fixed unit, connect the devices serial cable to the serial port RS485 and to the PC. You need a RS485 or RS232 converter to USB, depending from the laptop you are using.



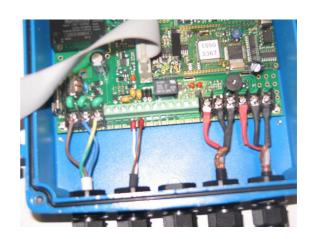


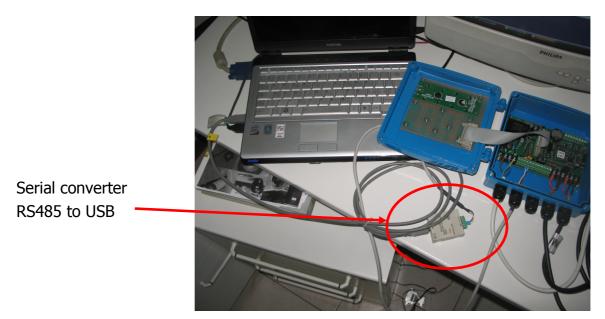

For portable unit, connect the devices serial cable to the serial port RS232 and to the PC.







Pag. 105 di










In this particular case we used an RS232/USB converter. It was connected with a short cable to a PC's USB port.





2.3 Connection software between the PC & the TTFM100 series

Start the Hyper Terminal application for Windows[©] XP[©] It will display:

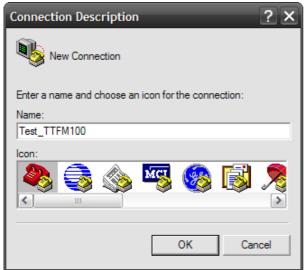

In the connection using set choose "COM7". (COM7 is valid for this example your port may be different).




In this example we call the connection "Test_TTFM100".

Click on "OK" the follow picture is about the connection to.




In the next picture you must set the same parameter as in the wall mounting or in portable unit.








Usually the communication parameters configuration of COM port is like in the side picture.

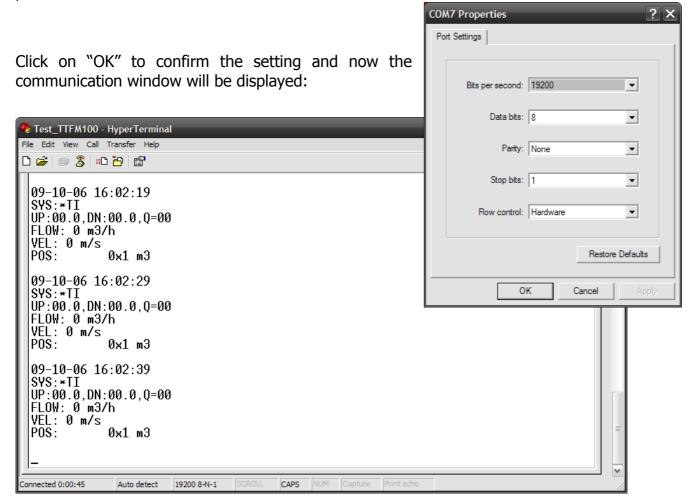

Please check during the operation, the status of communication:



In the example the device is not connected to the measuring point, as stated by the parameters:







All the parameters indicate "0" (zero) and the "System status" indicates errors, SYS:*TI.


2.4 Data logging in .txt - TEXT FORMAT

The Hyper Terminal program permits to log the TTFM100 data in a .txt file. Please proceed as follows.

First of all it is necessary to create a folder (directory) into which the files will be saved.


It should be possible to create this folder during the data logging settings, but the program already creates a folder itself:

Click on "Transfer" on the menu bar, and then click on "Capture Text".

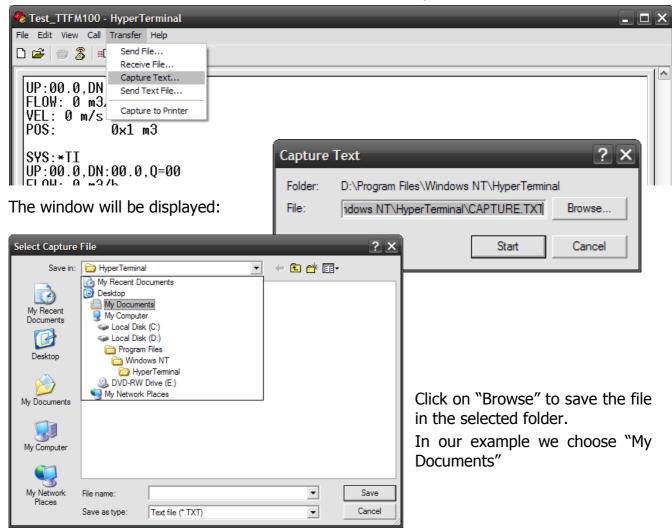






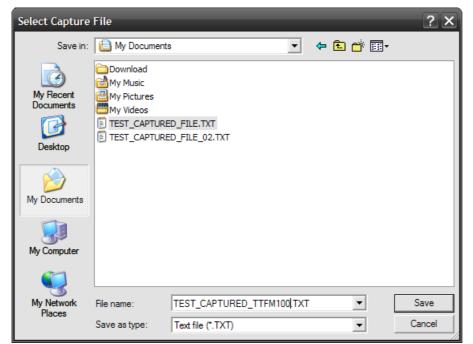


Click on "Save" the following window will be displayed:

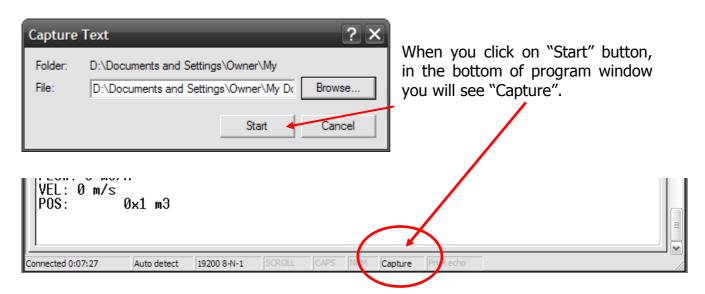


Now it is necessary to let the PC log the data for the needed time.

Once the data are logged, the user could stop the data logging by clicking on "Stop", as indicated in the following window:







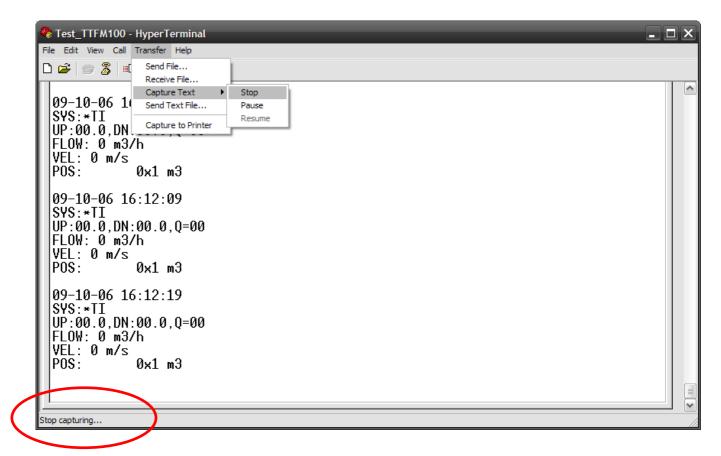



Exit this program as the other Windows $^{\! \tiny{\textcircled{\tiny C}}}$ XP $^{\! \tiny{\textcircled{\tiny C}}}$ programs.

3. How to use Excel® to read the .txt data

The following paragraph will only give a general idea on how to manage the data that have been logged with the previous indicated functions.






3.1 How to import .TXT files in Excel®

The user who wants to use this option must have a minimum Excel[©] knowledge, so all the procedures of opening and searching for files in the PC directories must be known.

Start the program and open a logged file (this file should have been logged during a regular TTFM100 functioning). The following example uses a file called TEST_CAPTURED_FILE.TXT. Did you remember in the last example we have used "My Documents" folder to store the captured file.

Attention: in order to display that file, please select "All files" (*.*).

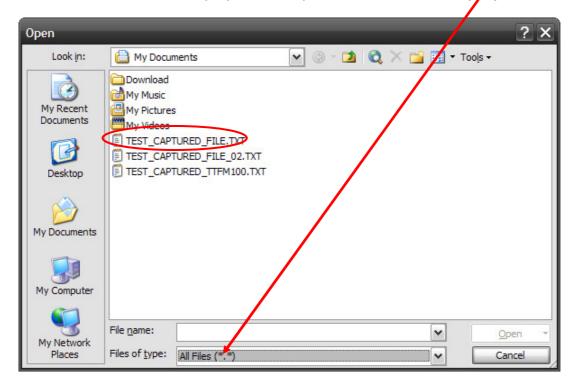







Pag. 112 di 126


The following "Text Import Wizard" window will appear: Choose "Windows (ANSI)

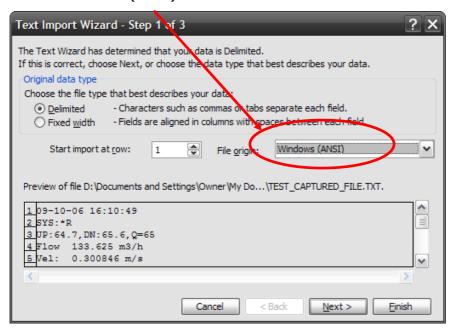

Click on "Next>" and it will display:

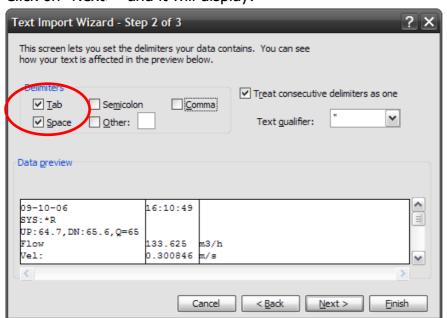


Please pay attention to choose "Tab" and "Space" tag and click on "Next>" button. Now it displays:











Pag. 113 di 126

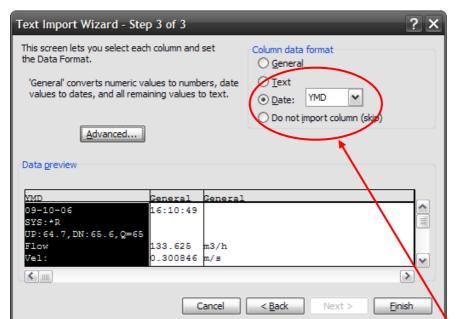

In this window it is necessary to click on "Advanced..." button.

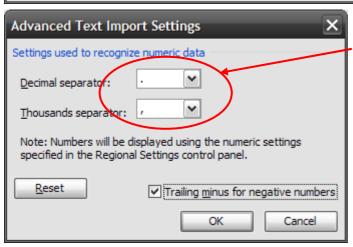


This window requires the decimal separator to be defined as dot "." and the thousands separator as comma ",". Click on OK button.

Go back to the previous window and set the data format in order to have a correct import. Select YMG that means year — month — day. Then click on "Finish" to complete the data import.







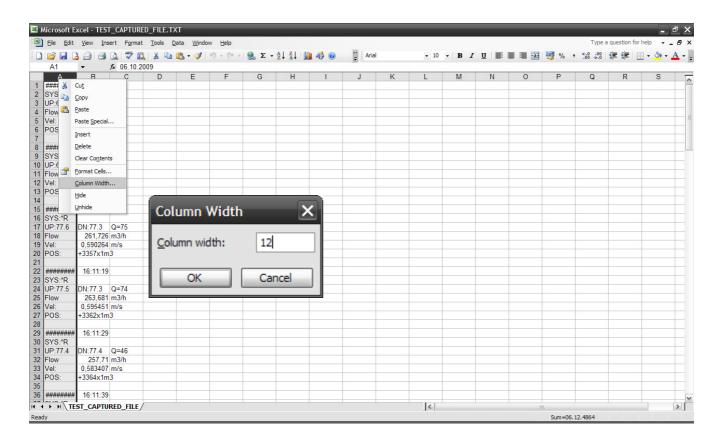

It is possible to change the columns width in order to display the date correctly. Click with the mouse right key on "Column A" and then click on "Column Width" and set it to 12 (for example).

It is necessary to re-elaborate the data because of the disposition in column and lines. In fact it does not permit to create a reliable bar graph of the desired measures.


The menu called "Data" helps the user to extract data, for example: the flow rate is the temporary date hour: minute: sec (h: m: s).

3.2 An example of Flow rate Bar graph


Select the first 3 columns "A-B-C" and click on "Automatic Filter" as follows:





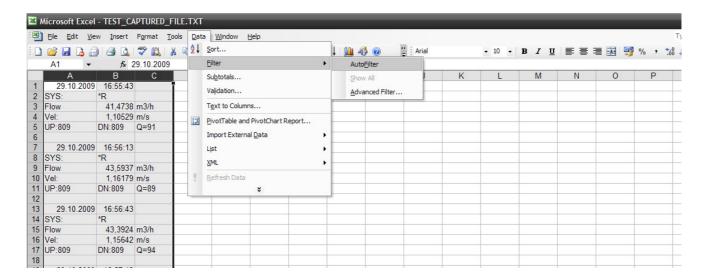


3 tags will appear on the upper right corner of each column:

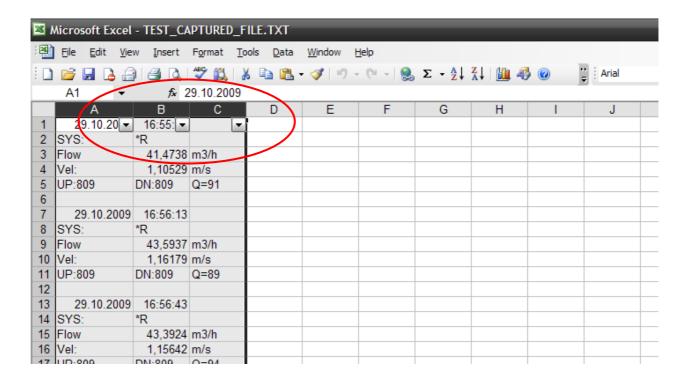






Click on the first tag and select the acquisition date line (it is assumed that the day is the same for all the columns!!).

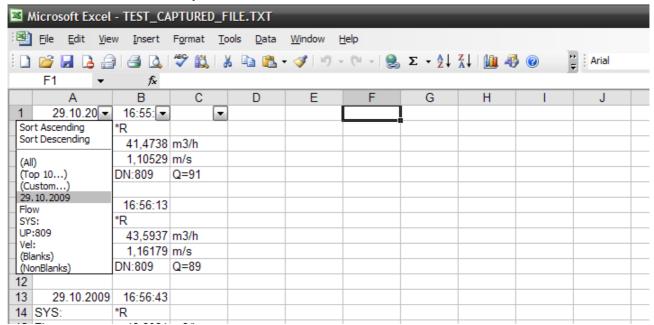

Excel will now extract the data into the lines according to the searching criteria.

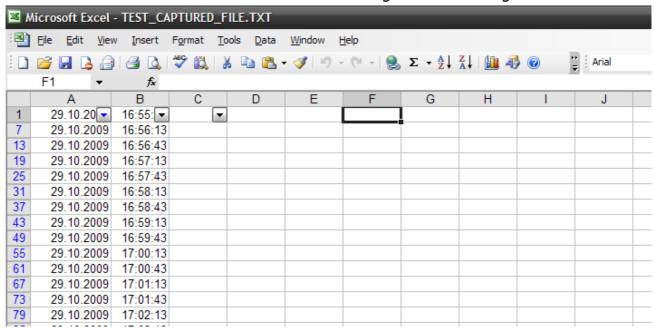


The date is the one referring to the hour in which the flow rate was logged.






During the text file import, Excel generated only one sheet into the folder, but at least another sheet is needed in order to manage this data extraction.

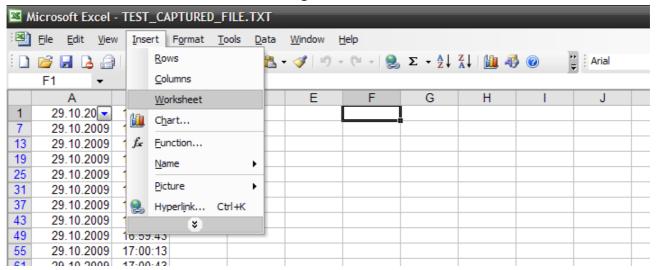


Click on "Insert", click on "Worksheet" and a new sheet will appear, named "Sheet 1". Return to the original sheet. Select the data into the hour column, and copy them.









Pag. 118 di

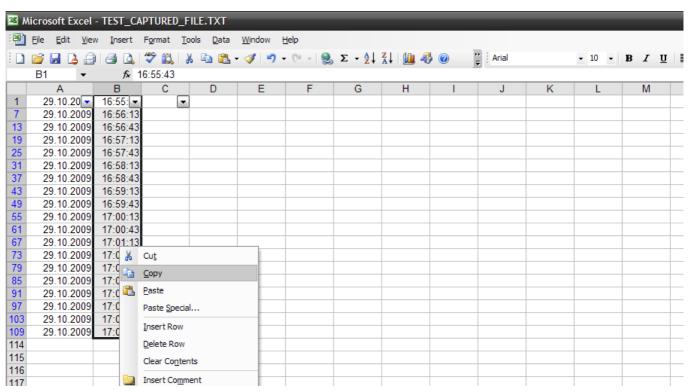

Go to sheet 1 and paste the copied data.

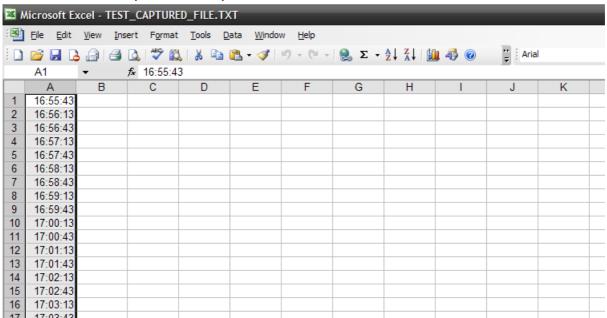

Now the acquisition time data are ok, but the flow data are still missing.








Pag. 119 di 126

Go back to the original sheet and click on the first tag, selecting Flow.

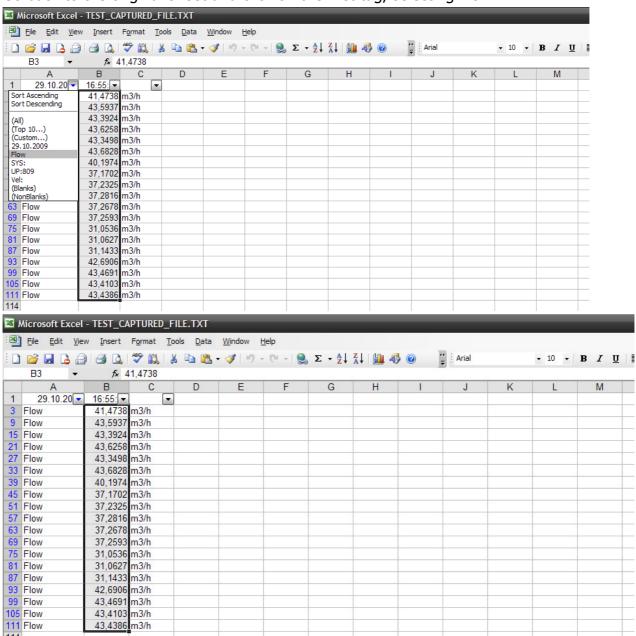


Now the B column will display the flow data.

The C column will display the flow rate engineering units.


Select and copy the flow data, as done for the time data, and paste it in "Sheet 1"








Pag. 120 di 126

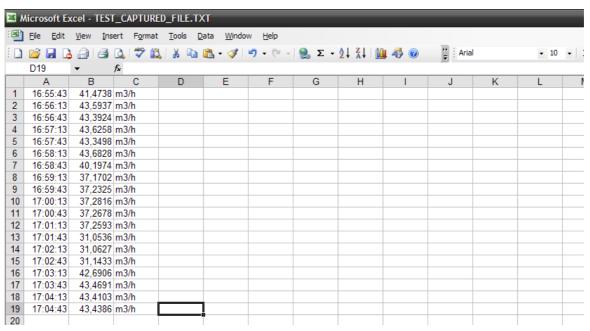


Now the data for the X axe and Y axe of the graph are complete.

Select the 2 group of data:

Go to "Insert", "Chart"

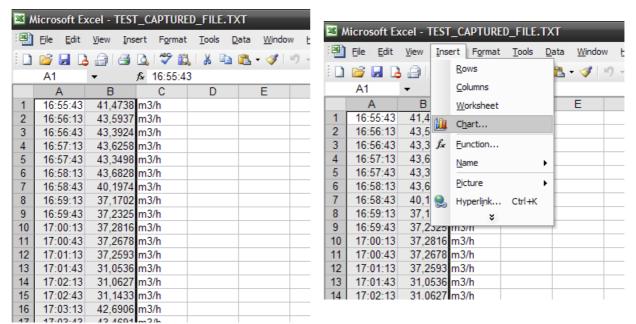


Now the type of Chart should be selected. Go into the Chart Wizard selection table and choose, for example, "XY (Scatter)" and then click on "Next" button.











Pag. 121 di 126

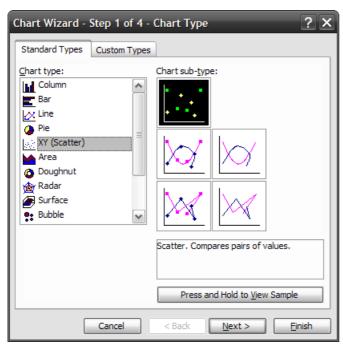


It is possible to see the type of chart displaying

the time flow rate. Click on "Next" button.

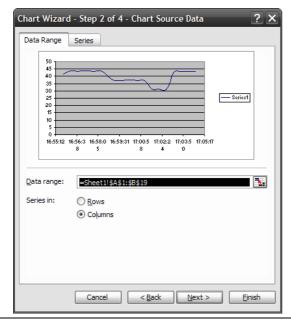


The following window will be displayed:

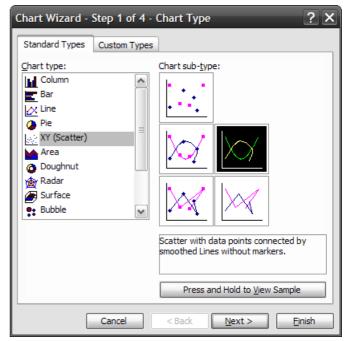


B.M. Tecnologie Industriali Via Praimbole 13 35010 LIMENA (PD) Cod.Fis./P.Iva IT02459940280








Pag. 122 di 126

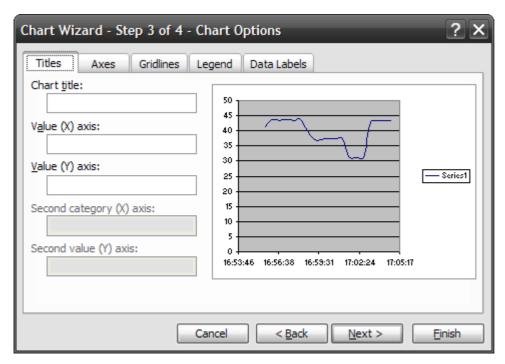

It is possible to scroll all the display's options or go directly to the 4th screen.

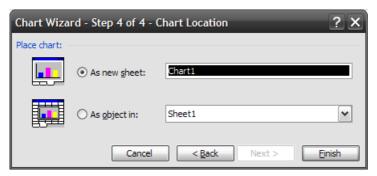


Click on "Next>". The last window will be displayed:

It is suggested to create the chart into a new sheet, Chart1 in the example windows.

Then Click on "Finish".






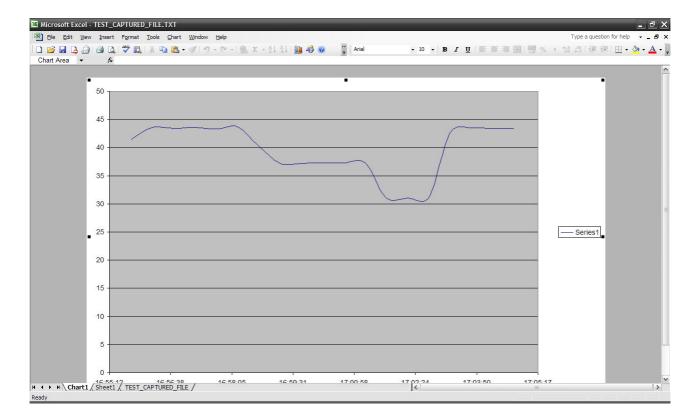

Now the final graph will be displayed.





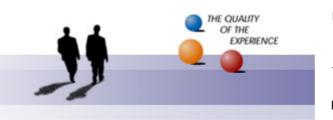

Pag. 124 di

4. EC- DECLARATION OF CONFORMITY

B.M. TECNOLOGIE INDUSTRIALI

hereby certifies

THAT THE DEVICES THIS MANUAL REFERS TO ARE IN CONFORMITY WITH APPLICABLE EUROPEAN DIRECTIVES:

89/336/EEC-EMC

73/23/EEC- LOW VOLTAGE

APPLIED STANDARDS:

EN50081:1992

BS EN61010-1:1993







Pag. 125 di 126





Management system as per EN ISO 9001 : 2000

In accordance with TÜV NORD CERT procedures, it is hereby certified that

B.M. Tecnologie Industriali S.r.l.

Via Praimbole, 13 35010 Limena (PD) Italy

applies a management system in line with the above standard for the following scope

Design, assembly and installation of industrial automation systems. Sale, assembly and installation of industrial automation systems.

Gertificate Registration No. 44 100 090264 Audit Report No. 3504 3619 Valid until 2010-11-15

G. Brantis am Gertification Body at TOV NORD CERT GRADH

Essen, 2009-05-20

This certification was conducted in accordance with the TÜV NORD CERT auditing and certification pracedures and is subject to regular surveillance audits.

TÜV NORD CERT GMBH

Langemarckstrasse 20

45141 Essen

mon tren-hond-rest dom




B.M. Tecnologie Industriali Via Praimbole 13 35010 LIMENA (PD) Cod.Fis./P.Iva IT02459940280



Tel. +39 (0) 49 884.16.51 Fax +39 (0) 49 884.16.54 E-Mail bm@bmtecnologie.it Web www.bmtecnologie.it



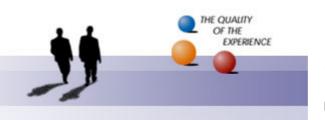

Pag. 126 di

Because of B.M. Tecnologie Industriali's policy of improving their products, the TTFM100 series, would be revised and improved.

Please inform us about misunderstandings or errors which you may find in this manual comparing it to the device you bought.

Do not hesitate to contact us to suggest how to improve our devices, thank You.

B.M. Tecnologie Industriali S.r.l. – Technical Dept.

B.M. Tecnologie Industriali s.r.l.

Via Praimbole, 13 – 35010 LIMENA (PD) – ITALY

Tel. 0039.049.8841651 – Fax 0039.049.8841654

E-Mail bm@bmtecnologie.it - Web www.bmtecnologie.it

