

www.greyline.com

USER'S GUIDE

Installation & Operation Instructions

Transit Time Flow Meter

Model TTFM 6.1

Manual Series A.1.8

Note: This page has been left blank intentionally.



INDEX

CONNECTIONS	4
KEYPAD SYSTEM	6
MENU SYSTEM	7
ICONS	8
MESSAGE ICON	9
STATUS	9
PASSWORD1	1
MENU SELECTIONS 1	1
UNITS/MODE	2
SET UP 1-	4
CALIBRATION	7
RELAY PARAMETERS	9
DATA LOGGING	0
COMMUNICATION (OPTIONAL)	2
SPECIAL FUNCTIONS	4
TYPICAL SE16B SENSOR INSTALLATION	7
TYPICAL SE16A SENSOR INSTALLATION	8
SENSOR MOUNTING	2
2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B TMK-B1 KIT	3
1 CROSS INSTALLATION OVERVIEW – SE16B TRANSDUCERS TMK-B1 KIT	7
2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B TRANSDUCERS TMK-B21 OR TMK-B22	KIT 44
1 CROSS INSTALLATION OVERVIEW – SE16B TRANSDUCERS TMK-B21 OR TMK-B22 KIT4	8
2 OR 4 CROSS INSTALLATION OVERVIEW – SE16A TRANSDUCERS TMK-A1 KIT	5
SENSOR MOUNTING/COUPLING RECOMMENDATIONS	8
ENCLOSURE INSTALLATION	9
FIELD TROUBLESHOOTING	0
COMMON QUESTIONS AND ANSWERS	3
APPLICATIONS HOTLINE	5
PRODUCT RETURN PROCEDURE	5
SPECIFICATIONS	
APPENDIX A - CONVERSION TABLE	1
PIPE CHARTS	2
APPENDIX C – LIQUID SPEED OF SOUND	7
APPENDIX D	4

IMPORTANT NOTE: This instrument is manufactured and calibrated to meet product specifications. Please read this manual carefully before installation and operation. Any unauthorized repairs or modifications may result in a suspension of the warranty. If this product is not used as specified by the manufacturer, protection may be impaired.

Available in Adobe Acrobat pdf format



CONNECTIONS:

POWER INPUT: The standard model requires AC power input between 100 to 240 VAC 50/60Hz 10VA. No adjustments are necessary for voltages within this range. Connect L (Live) N (Neutral) and AC Ground.

Optional DC input model requires 9-32 VDC/10 Watts. Connect to + and - terminals.

Optional Thermostat and Heater modules are available rated for specifically 115 VAC or specifically 230 VAC.

IMPORTANT NOTE: To comply with electrical safety standards, AC power input and relay connection wires must have conduit entry to the instrument enclosure. Installation requires a switch, overcurrent fuse or circuit breaker in the building (in close proximity to the equipment) that is marked as the disconnect switch.




Risk of electric shock. Loosen cover screw to access connections. Only qualified personnel should access connections.

Note: Use of instrumentation over 40°C ambient requires special field wiring.

Note: Some models feature a user replaceable fuse. Fuse is 2 Amp 250V (T2AL250V), located on the power supply.



100-240 VAC Meter CONNECTIONS

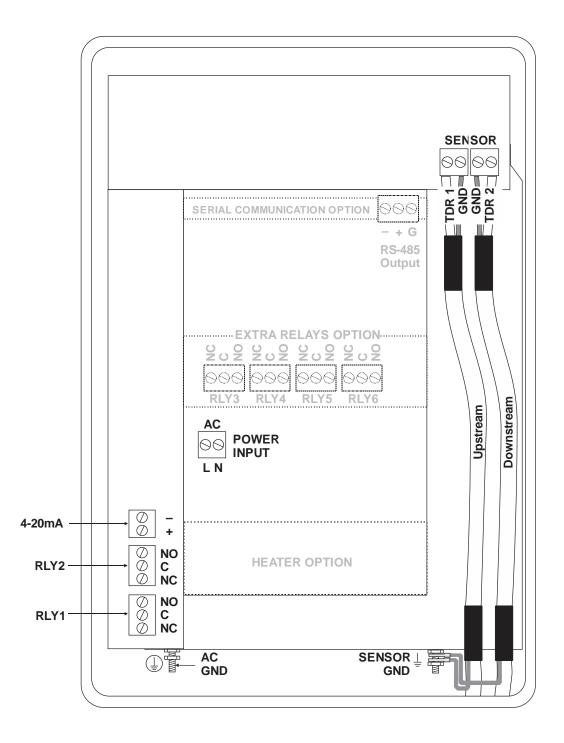





KEYPAD SYSTEM


The diagram on page 7 shows the TTFM 6.1 menu system. Arrows show the four directions to leave a menu box. Pressing a corresponding keypad arrow will move to the next item in the direction shown. Move the cursor (highlighted) under numerals and increase or decrease numerals with the \clubsuit and \clubsuit keys.

To store calibration values permanently (even through power interruptions), press the \checkmark button.

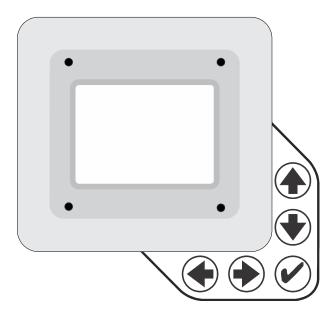






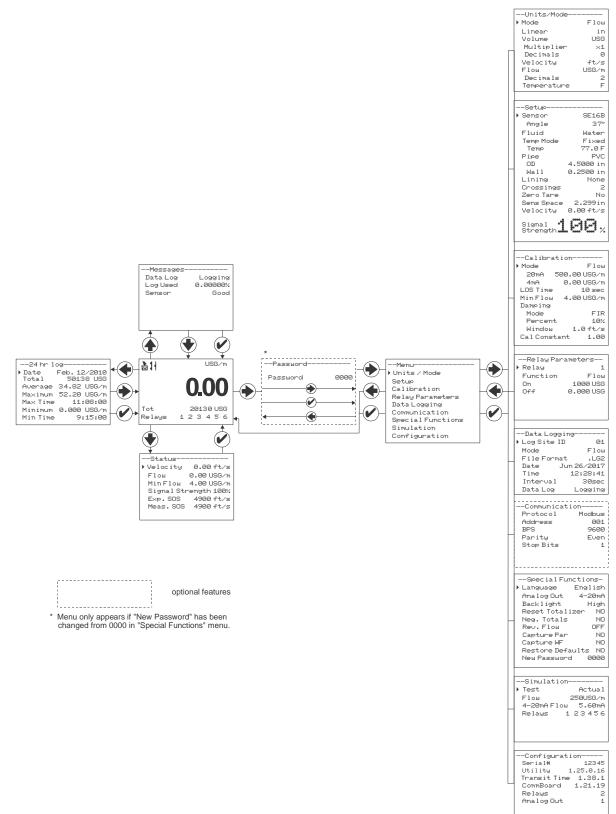



TTFM 6.1 Transit Time Flow Meter

ICONS

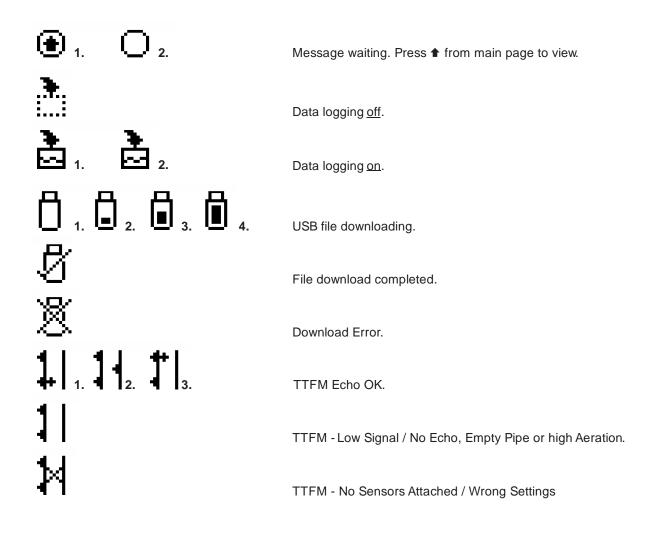





Messages Data Log Log Used Sensor	Stopped 0.00000 % Good

MAIN DISPLAY

The Main Display shows the units selected from the Units/Mode menu, flow rate or velocity rate being measured, totalizer, totalizer multiplier, and relay states. The TTFM 6.1 will go to this display after start-up.

MESSAGE ICON

Status	
▶ Velocity	0.00ft/s
Flow	0.00 USG/m
MinFlow	4.00 USG/m
Signal St	rength 100%
Exp.SOS	4900 ft/s
Meas.SOS	4900 ft/s

STATUS

Press \clubsuit from the Main Display to view Status of the measurement. Press \checkmark to return to the Main Display.

Velocity	Displays flow velocity in ft/s or m/s, selected in the Units/Mode menu.
Flow	Displays flow rate in units selected in the Units/Mode menu. A list of flow rate units is provided in the Units/Mode section of the manual.
MinFlow	Displays a read-only value for the minimum flow cutoff, in units which match the Flow selection. Measured flow rates below the Min Flow will result in the displayed flow rate on the LCD display to be 0.0. This parameter is used to suppress electrical noise at zero flow conditions, and it is typically set to the flow rate equivalent of 0.1 ft/sec in the programmed pipe size. The Min Flow can be adjusted in the Calibration menu.
Signal Strength	Displays magnitude of signal being received by the ultrasonic sensors. 100% is the ideal signal strength. Signal strengths less than 100% could indicate poor pipe conditions (corrosion), highly aerated water, or programmed setup parameters which don't closely match field conditions. Consideration should be made to use 1-cross installation method in such cases, if not already using it.



Status (cont.)

Status Velocity 0.00ft/s Flow 0.00USG/m MinFlow 4.00USG/m SignalStrength100% Exp.SOS 4900ft/s Meas.SOS 4900ft/s		Displays the expected fluid speed of sound measurement, in units that match the Velocity. The expected speed of sound is based on the pipe, fluid, and temperature selection in the Setup menu.
---	--	--

Meas. SOS Displays the measured fluid speed of sound, in units that

match Exp. SOS. The meter calculates this value based on the time it takes for the signal to arrive from one transducer to another. Large differences between expected and measured speed of sound (> 10%) typically indicate an error in the setup of the instrument. Verify the following are correct in the Setup menu and with the physical installation of the transducers:

- Pipe Material
- Pipe OD
- Pipe Wall Thickness
- Liner Type
- Liner Thickness
- Fluid Type
- Fluid Temperature
- Crossings
- Separation Distance




24 hr log		
▶Date	Feb. 12/2010	
Total	50138 USG	
Average	34.82 USG∕m	
Maximum	52.20 USG/m	
Max Time	11:08:00	
Minimum	0.000 USG/m	
Min Time	9:15:00	

24 HR LOG

Press \blacklozenge from the Main Display to view a formatted flow report. Press \clubsuit to scroll down one day or repeatedly to scroll to a specific date. Up to 365 days will be stored. Newest date will overwrite the oldest. Press \checkmark to return to the Main Display.

IMPORTANT: Inserting a USB drive into the meter while on this screen will transfer 24 HR Log data to the USB drive in .csv format.



PASSWORD

The Password (a number from 0000 to 9999) prevents unauthorized access to the Calibration menu.

From the Main Display press the \Rightarrow key to get to Password. Factory default password is 0000 and if it has not been changed, this screen will be bypassed completely.

A new password can be stored by going to the Special Functions New Password menu.

If a user password is required, press \Rightarrow to place the cursor under the first digit and \clubsuit or \clubsuit to set the number, then \Rightarrow to the second digit, etc. Press \Rightarrow or \checkmark to proceed to the Menu Selections screen.

MENU SELECTIONS

The Menu selections page is used to navigate to specific menus which are described in more detail on the following pages.

Press \clubsuit or \clubsuit to navigate to different menus, and \clubsuit to enter the selected menu.

--Menu------> Units / Mode Setup Calibration Relay Parameters Data Logging Communication Special Functions Simulation Configuration



Units/Mode	
▶ Mode	Flow
Linear	in
Volume	USG
Multiplier	$\times 1$
Decimals	0
Velocity	ft/s
Flow	USG/m
Decimals	2
Temperature	F

UNITS/MODE

At Mode, press the \rightarrow and then the \uparrow or \clubsuit to select Flow or Velocity. Flow mode displays the flow rate in engineering units (e.g. gpm, litres/sec, etc.) Press the \checkmark to store your selection then the \clubsuit to the next menu item.

At $\ \ inear$ press the $\ \ key$ and then the $\ \ or \ \ vot select your units of measurement. The Linear units define what units the pipe dimensions and sensor spacing will be displayed in. Typically inches or mm is selected. Press the <math>\ \ vot store$ your selection then the $\ \ vot$ to the next menu item.

At Volume, press the \Rightarrow and then the \uparrow or \clubsuit to select units for volume. Note: "bbl" denotes US oil barrels. Press the \checkmark to store your selection then the \clubsuit to the next menu item.

At Multiplier, press the \Rightarrow and then the \uparrow or \clubsuit to select the totalizer multiplier. Multipliers are used when resolution down to single digit is not required, or when you don't want to convert from gallons to thousands of gallons, as an example. Press \checkmark to store your selection then \clubsuit to the next menu item.

At Dec imals (Volume), press the \Rightarrow and then the \uparrow or \clubsuit to select the number of decimal points to be present on the totalizer display on the LCD screen. Default = 0. Options = 0, 1, 2. Press the \checkmark to store your selection then the \clubsuit to the next menu item.

At $\forall elocity$, press the \Rightarrow and then the \uparrow or \clubsuit to select the engineering units for flow velocity and sonic velocity of the fluid. Press \checkmark to store your selection then \clubsuit to the next menu item.



Units/Mode	
▶ Mode	Flow
Linear	in
Volume	USG
Multiplier	×1
Velocity	ft/s
Flow	USG∕m
Temperature	F

UNITS/MODE (cont.)

At Flow, press the \Rightarrow and then the \uparrow or \clubsuit to select the engineering units for flow rate. Press \checkmark to store your selection then \clubsuit to the next menu item.

Available Flow Rate Engineering Units:

Abbreviation	Description	Abbreviation	Description
USG/d	US gallons per day	L/d	liters per day
USG/h	US gallons per hour	L/h	liters per hour
USG/m	US gallons per minute	L/m	liters per minute
USG/s	US gallons per second	L/s	liters per second
ft ³ /d	cubic feet per day	m ³ /d	cubic meters per day
ft ³ /h	cubic feet per hour	m ³ /h	cubic meters per hour
ft ³ /m	cubic feet per minute	m ³ /m	cubic meters per minute
ft ³ /s	cubic feet per second	m ³ /s	cubic meters per second
bbl/d	barrels per day (1 $bbl = 42 USG$)	IG/d	Imperial gallons per day
bbl/h	barrels per hour $(1 \text{ bbl} = 42 \text{ USG})$	IG/d	Imperial gallons per day
bbl/m	barrels per minute (1 $bbl = 42 USG$)	IG/d	Imperial gallons per day
bbl/d	barrels per second (1 $bbl = 42 USG$)	IG/d	Imperial gallons per day
USMG/d	US million gallons per day	IMG/d	Imperial million gallons per day
USMG/h	US million gallons per hour	IMG/h	Imperial million gallons per hour
USMG/m	US million gallons per minute	IMG/m	Imperial million gallons per minute
USMG/s	US million gallons per second	IMG/s	Imperial million gallons per second

At Dec imals (Flow), press the \clubsuit and then the \clubsuit or \clubsuit to select the number of decimal points to be present on the flow rate display on the LCD screen. Default = 2. Options = 0, 1, 2. Press the \checkmark to store your selection then the \clubsuit to the next menu item.

At Temperature, press the \Rightarrow and then the \uparrow or \clubsuit to select units for temperature. Press the \checkmark to store your selection then the \uparrow to go back to another menu item, or \blacklozenge to exit back to the Menu Selection screen.



Contrara.	
Setup	
▶ Sensor	SE16B
Angle	37°
Fluid	Water
Temp Mode	Fixed
Temp	77.0F
Pipe	PVC
OD	4.5000 in
Wall	0.2500 in
Lining	None
Crossings	2
Zero Tare	No
Sens Space	2.299in
Velocity	0.00 ft/s
Signal • Strength	.99%

SET UP

Press \clubsuit or \clubsuit to position curser at Setup, and \clubsuit to enter. Use \clubsuit or \clubsuit to position cursor before each menu item and \clubsuit to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

Sensor Choose SE16B or SE16A, depending on transducers connected to TTFM 6.1.

For SE16B only, select angle which matches the transducer pair connected to the TTFM. Options: 35, 37, 39, and 41. Angle is determined by the part number on the SE16-B transducer label. Guide:

Part Number on SE16-B Label	Corresponding Transducer Angle
SE16-B-35	35
SE16-B-37	37
SE16-B-39	39
SE16-B-41	41

- Fluid Select fluid type.
 - V = 1 @ 25 C When Fluid = Other, enter the fluid velocity at 25C from table or other reference. Engineering units may be m/s or ft/s depending on Units menu programming.
- $\frac{dV}{C}$ When Fluid = Other, Enter fluid velocity adjustment factor over change in temperature in units of m/s or ft/s per °C.
- Temp Mode Choose Fixed.
- Temp Enter fluid operating temperature in displayed engineering units.
- Pipe Select pipe material.
 - Pipe VelWhen Pipe = Other, enter pipe material speed of sound (consult
factory).
 - □D Highlight the digits and then **↑** or **↓** to change the numbers and decimal point. Pipe OD should be entered as the exact outside diameter of the pipe where the sensor is mounted. Refer to the Pipe Charts Appendix in this manual for outside diameter of common pipe types and sizes.
- Wall 1Enter pipe wall thickness. Pipe wall thickness should be entered
as the exact wall thickness of the pipe where the sensor is
mounted. Refer to the Pipe Charts Appendix in
this manual for wall thicknesses of common pipe types and
sizes.



Setup	
▶ Sensor	SE16B
Angle	37°
Fluid	Water
Temp Mode	Fixed
Temp	77.0F
Pipe	PVC
OD	4.5000 in
Wall	0.2500 in
Lining	None
Crossings	2
Zero Tare	No
Sens Space	2.299in
Velocity	0.00 ft/s
Signal • Strength	.99%

Lining Select liner material.


SET UP (cont.)

Vel

- When Lining = Other, enter speed of sound of liner (consult factory).
- Thick When Lining \neq None, enter liner thickness.

Crossings

Crossings 1 = Z mounting

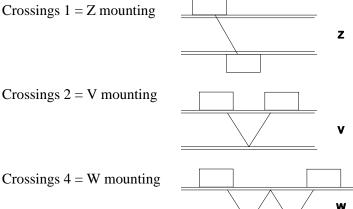

Nominal Pipe Size, Inches	Recommended Crossings
0.5-1.5	Crossings = 4
2-24	Crossings = 2
> 24	Crossings = 1

Older pipes are often degraded or scaled on the inside. These conditions can hinder the ability to receive a strong signal when Crossings = 2. Greyline suggests starting with Crossings = 1 in cases such as these.

Zero Tare Used to calibrate zero-flow measured by the TTFM 6.1 in process. Flow in the pipe should be confirmed as 0 before enabling, or significant errors in flow accuracy could occur.

> Set Calibration/Damping to 0%, and under no flow conditions and with a full pipe, select Yes to force readings to zero.

- Sens Space After sensor, angle, fluid, and pipe material are defined, this displays the calculated sensor spacing. Also called the separation distance. The sensors will be set to this dimension when installed on the pipe, as described later in this manual.
- Velocitu Displays the measured velocity after the sensors have been connected at the specified separation distance.



Setup	
▶ Sensor	SE16B
Angle	37°
Fluid	Water
Temp Mode	Fixed
Temp	77.0F
Pipe	PVC
OD	4.5000 in
Wall	0.2500 in
Lining	None
Crossings	2
Zero Tare	No
Sens Space	2.299in
Velocity	0.00 ft/s
Signal • Strength	.98%

SET UP (cont.)

Signal Strength Displays magnitude of signal being received by the ultrasonic sensor. Should be 100% under ideal operating conditions. Signal strengths less than 100% do not indicate that the meter is not reliable, however, the meter may be more susceptible to complete signal loss should process conditions like entrapped air worsen. When signal strength is less than 100%, consideration should be made to using 1-cross mounting method if this is not the current mounting mode.



Calibration	
▶ Mode	Flow
20mA 5	500.00 USG/m
4mA	0.00 USG/m
LOS Time	10 sec
MinFlow	4.00 USG/m
Damping	
Mode	FIR
Percent	10%
Window	1.0 ft/s
Cal Const	ant 1.00

CALIBRATION

Press \clubsuit or \clubsuit to position curser at Calibration menu, and \clubsuit to enter. Use \clubsuit or \clubsuit to position cursor before each menu item and \Rightarrow to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

Mode Displays the Mode which was selected in the Units/Mode menu. This is read-only. 20mA Press \Rightarrow then \clubsuit or \clubsuit to change the numbers and decimal point position. Use this menu to set the corresponding flow rate that will be represented by 20mA analog output. If maximum flow is unknown, enter an estimated flow rate and observe actual flow to determine the correct maximum value. Any velocity or flow rate up to +40 ft/sec (12.0 m/sec) may be selected. 4mA Press \Rightarrow then \clubsuit or \clubsuit to set the flow rate corresponding to 4mA analog output. This setting may be left at zero or can be raised to any value less than the 20mA setting, or lowered to any velocity or corresponding flow rate down to -40 ft/sec (-12 m/sec). LOS Time Use LOS Time to suppress intermittent loss of signal. Example: systems with high concentrations of undissolved gasses will cause fluctuations in signal strength when the gasses move past the ultrasonic signal. If a complete loss of signal is experienced, the TTFM 6.1 will hold the last valid reading for the duration of the LOS Time. If the signal strength returns before the LOS Time is expired, because the ultrasonic signal is no longer being impeded, the meter will return to normal operation automatically. If signal strength does not return after the LOS Time has expired, then the meter will report zero flow on the LCD display and outputs, and produce a Low Signal alarm. Default LOS Time is 30 seconds, and the value can be set between 0 and 99 seconds. MinFlow Flow rates below this setting will be displayed as zero flow. Default flow rate is ~ 0.1 ft/sec for the pipe size programmed in the Setup menu.



Calibration	CALIBRATION	(cont.)
▶Mode Flow		
20ma 500.00 USG/m 4ma 0.00 USG/m	Damping	
LOS Time 10 sec		
MinFlow 4.00 USG/m	Mode	Choose between OFF, FIR (Default), or LOW PASS.
Damping Mode FIR		
Percent 10%		When measured flows are outside the Window of the running
Window 1.0ft/s CalConstant 1.00		average, the FIR filter will reduce the damping average so that a fast response can be made to the sudden change in flow rate.
		a fast response can be made to the sudden change in now fate.
		The LOW PASS filter will ignore measured flow rates outside
		the Window, while holding the running average, until there are
		enough data points outside the Window to cause a step-
		response to the new measured value.
		Within a second floor and still in the With loss of the second second
		While measured flows are within the Window of the running average, both the FIR and LOW PASS filter behave the same.
		average, both the FIK and LOW FASS filter behave the same.

- PercentHigher percentages increase the number of measurements
which are averaged together to produce a stable flow reading.
Higher percentages also increase the time it takes for the meter
to make a step-response to the measured flow rate outside the
Window in the LOW PASS Mode.
- WindowDefines the Window around the running average, in units of
Velocity set in the Units/Mode menu. Measurements made
inside the Window are added to the running average, and
measurements outside the Window effect the response of the
meter as described in the Mode section.
- Cal Calibration constant defined when the TTFM was calibrated at the Greyline factory.

Press \checkmark to return to Menu Selections.



Relay Parameters		
▶ Relay	1	
Function	Flow	
On	1000 USG	
Off	0.000 USG	

RELAY PARAMETERS

Press \clubsuit or \clubsuit to position curser at Relay Parameters, and \clubsuit to enter. Use \clubsuit or \clubsuit to position cursor before each menu item and \clubsuit to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

- RelayPress ⇒ and ↓ or ↑ to select a corresponding relay number
(2 relays are standard, 4 additional are optional).FunctionPress ♦ or ↑ to select Off, On, Pulse,
Direction, or Flow.PulsePress ♦ and set digits to the flow volume increment required
 - Press and set digits to the flow volume increment required between relay pulses. Use this feature for remote samplers, chlorinators or totalizers. Minimum time between pulses is 2.25 seconds and pulse duration is 350 milliseconds.

Return to Relay and change settings for each relay number.

Press ✓ to return to Menu Selections.

- Direction When flow is in the positive direction, the relay will be disengaged, when flow is negative, the relay engages. Note: Rev. Flow in the Special Functions menu must be ON or INVERT for this to work properly.
- Flow Mode Select Pump

Pump mode provides separate On/Off settings where the relay will energize at one flow rate and de-energize at another.

 \Box_{Γ} Highlight the numerals and press \clubsuit or \clubsuit to set digits to the required relay \Box_{Γ} set point.

Off set digits to the required Off set point.



Data Log	ging
▶Log Site 1	
	99
Mode	Flow Velocity
Set Date	
Set Time	11:27:40
Interval	10sec
	60min
	30min 15min
	10min
	5min
	2min 1min
	30sec
Log	Stop
	Start
	Delete

DATA LOGGING

Press \clubsuit or \clubsuit to position curser at Data Logging, and \clubsuit to enter. Use \clubsuit or \bigstar to position cursor before each menu item and \clubsuit to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

- Log Site ID Enter a number from 00 to 99. The site ID will become part of the downloaded file name to help distinguish downloads from different instruments. Press ✓ to store the setting.
- Mode Select Velocity (e.g. ft/sec or m/sec) or Flow (e.g. USGPM or l/sec). Press ✓ to store the setting. This setting cannot be changed after a log was started. To change, first stop the log, then change the mode.

FileFormat Choose .LG2 to download data in .lg2 format for viewing on Greyline Logger software. Choose .CSV to download data in .csv format for import directly to Excel. This menu option can be changed at any time without adversely affecting existing data.

- Date Press \Rightarrow , and \bigstar or \clubsuit to scroll and select Month, Day and Year. Press \checkmark to store the setting.
- TimePress \Rightarrow , and \bigstar or \clubsuit to select the current time in Hours,
Minutes and Seconds. Press \checkmark to store the setting.
- Interval Press or to select the logging interval. Press to store the setting. Greyline recommends choosing an interval which will give you as much resolution as required and no more. Choosing too often of an interval for what is required will result in larger data files, which may take a long time to download to USB. Reference page 18 for specific download times. In critical installations, data should be downloaded often.
- Data Log Stop, Start or Delete the log file. Press \clubsuit or \clubsuit to select Delete and \checkmark to delete the log file. Press \clubsuit or \clubsuit to select Start and \checkmark to start the logger.

Important Note: You <u>MUST</u> Delete an old log and Start a new log <u>AFTER</u> having made changes to Log Site ID, Mode, Date, Time and/or Interval for those changes to be applied.

Important Note: Changing any of the parameters in the Units/Mode menu will start a new log. It is recommended that you Delete and start a new log after changing any Units/Mode settings.



RETRIEVING LOG FILE

Plug a USB Flash Memory Drive (one is included with the TTFM 6.1) into the USB output port on the Panel of the meter. The instrument display will show the data download icon until the log file is transferred to the memory card. The USB flash drive may be removed when the icon for download successful appears.

Download file names will appear in this format:



Tag is set according to the Log Site ID entered in the instrument Data Logging menu.

Download letter will be A for the first download from an instrument. B for the second, then C etc. At the letter Z a - character will appear indicating that the maximum number of downloads for that instrument are on the USB flash drive. Older files can be erased or moved from the flash memory drive or a new memory drive can be used.

Note: Downloading files in .lg2 format will take approximately 35 seconds per 1% of internal log memory used.
Downloading files in .csv format will take approximately 8 minutes per 1% of internal log memory used.

OPENING .LG2 FILES

Install Greyline Logger on your PC or laptop. Select File/Open/Instrument Log (.log) to open the log file from your USB flash drive. Greyline Logger software is available on Greyline's website, <u>www.greyline.com</u>. Data can also be converted to .CSV via Greyline Logger software.

OPENING .CSV FILES

Use a datasheet program such as Microsoft Excel® to import data in a comma delimited format. Use Excel to manipulate or graph data.




Communication		
Protocol	Modibus	
Address	001	
BPS	9600	
Parity	Even	
Stop Bits	1	

COMMUNICATION (Optional)

Press \clubsuit or \clubsuit to position curser at Communication, and \clubsuit to enter. Use \clubsuit or \bigstar to position cursor before each menu item and \clubsuit to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

MODBUS Protocol Information:

Transceiver:	2-wire, half-duplex
Data format:	8 Data Bits
Floating Point Byt	e Order: ABCD
Termination:	Jumper JP1 selectable 120Ω resistor. TB1 & TB2 = OFF,
	TB2 & TB3 = ON
Biasing:	None

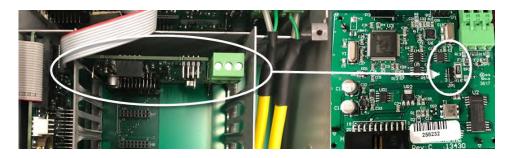

HART® (Highway Addressable Remote Transducer) Protocol Information:

HART Version: 7.0

Device Description Files:	DD files allow the user's handheld HART communicator to fully configure the TTFM 6.1 Greyline provides DD files for the Emerson 475 Communicator. The files are included in the USB drive provided with your TTFM 6.1 meter. You may also request the files from Greyline by calling or emailing us at <u>info@ greyline.com</u> . Warning: The TTFM 6.1 and associated DDs are pending certification from the Fieldcomm Group.
Connections:	HART Protocol uses a digital signal superimposed on the 4-20mA output. When the 4-20mA output of the TTFM 6.1 is connected with a load resistor (230Ω to 600Ω), the HART communicator can be connected on the loop in order to communicate.
Protocol	Choose MODBUS or HART.
Address (Modbus)	Device address for the TTFM. Valid range: 001-247 (Default: 001). This number should be unique across the bus. Press \clubsuit or \clubsuit to scroll, \clubsuit to select digits, and press \checkmark to store the setting.



Communication	
Protocol	Modibus
Address	001
BPS	9600
Parity	Even
Stop Bits	1

COMMUNICATION (Optional) (cont.)

BPS (Modbus)	Baud rate for the MODBUS communications. Press ★ or ↓ to select, and ✓ to store the setting. Options: 4800, 9600, 19200, 38400, 57600, 76800, and 115200 (Default: 9600).
Parity (Modbus)	Error checking parity for the MODBUS communications. Press \clubsuit or \clubsuit to select, and \checkmark to store the setting. Options: None, Even, and Odd (Default: Even).
Stop Bits (Modbus)	Press \clubsuit or \clubsuit to select, and \checkmark to store the setting. Options: 1 or 2 (Default: 1).

Note: The Modbus register table, and HART configuration instructions can be found in separate TTFM 6.1 Serial Communications Manual.



Special Functions-		
▶ Language Eng	lish	
AnalogOut 4-	20mA	
Backlight	High	
Reset Totalizer	NO	
Neg. Totals	NO	
Rev.Flow	OFF	
Capture Par	NO	
Capture WF	NO	
Restore Defaults	5 NO	
New Password	0000	

SPECIAL FUNCTIONS

Press \clubsuit or \clubsuit to position curser at Special Functions, and \clubsuit to enter. Use \clubsuit or \clubsuit to position cursor before each menu item and \clubsuit to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

Language	Select English, French or Spanish
Analog Out	Select 4-20mA or 0-5V mode for the analog output.
Backlight	Select High, Medium or Low for continuous backlight brightness.
	Select $K \in Hi / Lo$ for high backlight lasting 1 minute after a keypress, and then Lo backlight until a key is pressed again.
	Select Key High, Med or Low for backlight lasting 1 minute after a keypress and then backlight off until a key is pressed again.
Reset Totalizer	Select $\forall e \equiv$ to erase and restart the totalizer at zero.
Negative Totals	Select $\forall e \equiv$ to have reverse flow readings deducted from the totalizer. Select No to totalize forward flow only and ignore reverse flow.
Re∨.Flow	Select $\Box n$ to enable flow direction measurement. Select $\Box f f$ to disable flow direction measurement so that flow in either direction is displayed and output as positive values. Select Invert to invert the sense of the flow measurement.
Capture Par	This function captures the programming parameters in the meter. Select $\forall \in \exists$, wait for $\exists n \exists n \exists n t$ USB to appear, then insert a USB drive into the USB port to transfer the parameters. After Saving flashes, $\exists on =$ will appear on the screen, meaning it is safe to remove the USB,



SPECIAL FUNCTIONS (cont.)

Capture WF

Restore

Defaults

Special Function	ns-
▶ Language Engl	ish
Analog Out 4-2	ØmA
Backlight H	igh
Reset Totalizer	NO
Neg. Totals	NO
Rev.Flow	OFF
Capture Par	NO
Capture WF	NO
Restore Defaults	NO
New Password 0	000

This function should only be used when instructed by a Greyline representative to do so. The function captures the ultrasonic signal so that it can be evaluated by Greyline.

Select $\forall e \equiv$ to start the waveform download process. After pressing $\forall e \equiv$, the screen will flash Work ing for approximately 20 seconds, until the message Insrt USB appears. When Insrt USB is on the screen, connect a flash drive to the USB port on the front of the meter. The screen will flash Sauing for a couple seconds, and then return to Done. The waveform is now stored on your flash drive and ready to be sent to Greyline.

Select $\forall \Theta \equiv$ to erase all user settings and return the instrument to factory default settings. Note: does not reset factory calibration values.

New Password Select any number from 0000 to 9999. Default setting of 0000 will allow direct access to the calibration menus. Setting any password other than 0000 will require the password to be entered to access the calibration menus.

Press ✓ to return to Menu Selections.



Simulation				
▶Test	Actual			
Flow	250USG/m			
4-20mAFlow	5.60mA			
Relays 1 2	3456			

SIMULATION

Press \clubsuit or \clubsuit to position curser at Simulation, and \clubsuit to enter. Use \clubsuit or \clubsuit to position cursor before each menu item and \clubsuit to enter. When settings are completed press \checkmark to store and \checkmark again to return to the Main Menu.

Changes made in the Simulation menu exercise the 4-20mA output, digital display and control relays.


Simulate a Flow/Velocity reading. Press \Rightarrow and then \clubsuit or \bigstar to change the simulated output. Press \checkmark to begin simulation. The 4-20mA output and relay states will be displayed on the screen below.

Press the \checkmark to terminate simulation and return to the Menu Selections screen.





TTFM 6.1 Transit Time Flow Meter

TYPICAL SE16B SENSOR INSTALLATION

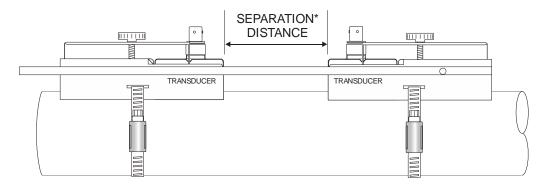

2 Cross Separation Distance



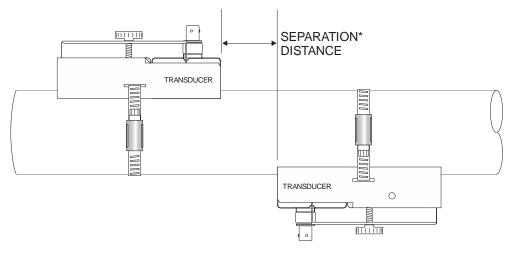


* Shown in 'Setup' menu after sensor, fluid and pipe parameters are entered.

TMK-B1 transducer mounting kit shown. Sensor spacing method is consistent with TMK-B21 and TMK-B22 kits, but the brackets will be different.



TYPICAL SE16A SENSOR INSTALLATION



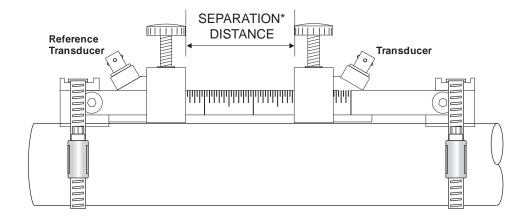

* Shown in 'Setup' menu after sensor, fluid and pipe parameters are entered.

Separation distance is measured from transducer face to transducer face. Reference transducer is placed flush to bracket.

Mount the supplied SE16A Series Transducers on pipes 0.5" / 15 mm OD or larger.




SE16B Pipe Preparation and Bracket Mounting

Prepare an area 2" wide by 4" long (50mm x 100mm) for each sensor bonding by removing loose paint, scale and rust. The objective of site preparation is to eliminate any discontinuity between the sensor and the pipe wall, which would prevent acoustical coupling. A sanding block is included with every meter to facilitate proper pipe preparation.


A Sensor Mounting Kit is supplied with each Greyline flow meter. It includes recommended coupling compound and a stainless steel mounting bracket with adjustable pipe straps. Use the Alignment Bar (included) to align sensor brackets for V and W mode mounting.

IMPORTANT: The SE16-B transit-time transducers have arrows on the top of them. These should face each other at installation.

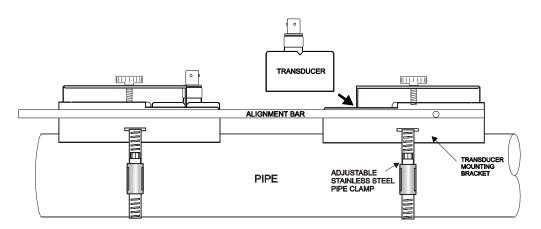

Mount the Mounting Bracket as illustrated on pipes 2" / 50 mm OD or larger. Stainless steel bands are included for mounting on pipes up to 30" / 750 mm OD.

Additional stainless steel bands (provided by customer) may be combined to mount on larger pipes. TMK-B1 Installation Kit shown.

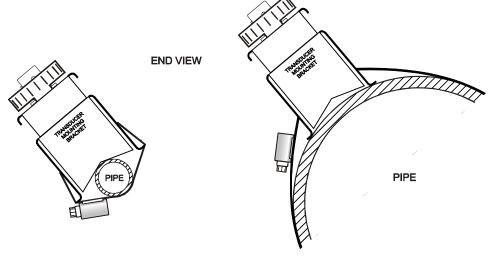






SE16A Pipe Preparation and Bracket Mounting

Prepare an area 2" wide by 10" long (50mm x 250mm) for the track mounting bracket by removing loose paint, scale and rust. The objective of site preparation is to eliminate any discontinuity between the sensor and the pipe wall, which would prevent acoustical coupling. A sanding block is included with every meter to facilitate proper pipe preparation.

A Sensor Mounting Kit is supplied with each Greyline flow meter. It includes recommended coupling compound and a stainless steel mounting bracket with adjustable pipe straps. Use the built-in ruler to easily measure separation distance between transducer faces.

IMPORTANT: The SE16-A transit-time transducers should be installed with the cable connections pointed away from each other, as shown in the drawing below.

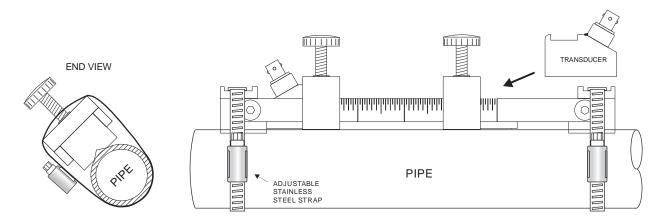

Mount the supplied SE16A Series Transducers on pipes 0.5" / 15 mm OD or larger.




SENSOR COUPLING

For permanent or temporary bonding, the following are recommended:


- a) Super Lube® (supplied) Additional supply: order Greyline Option CC-SL30 or your local home improvement store.
- b) Water-based sonic compound: Order Greyline Option CC30
- c) Electrocardiograph gel
- d) Petroleum gel (Vaseline)

The above are arranged in their order of preferred application. Option d is only good for temporary bonding at room temperature. DO NOT USE: Silicon RTV caulking compound (silicon rubber).




Use the pipe clamp and rail (supplied) as illustrated on previous page. Apply Super Lube® to the colored face of the sensor. A bead, similar to toothpaste on a toothbrush, is ideal. Do not overtighten (crush the sensor).

The sensor must be fixed securely to the pipe with coupling material between the sensor face and the pipe. Sensor installation with excessive coupling compound can result in gaps or voids in the coupling and cause errors or loss of signal. Insufficient coupling compound will create similar conditions.



Over time temporary coupling compounds (e.g. Petroleum Gel) may gradually sag away from the sensor resulting in reduced signal strength and finally complete loss of signal. Warm temperatures, moisture and vibration will accelerate this process. Super Lube® as supplied with the TTFM 6.1 (and available from Greyline Instruments or home improvement stores) is recommended for permanent installations.

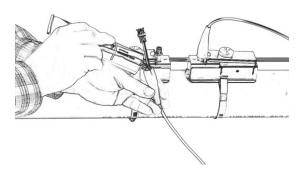

Transducer Installation in Wet Locations

The TTFM 6.1 Transit Time Flowmeter transducers are rated for accidental submersion up to 10 psi (0.75 bar). The flowmeter will continue to operate and measure flow accurately during periods of submergence. Plastic seal jackets on the cables must be filled with coupling compound to provide additional moisture protection for the BNC cable connectors.



SENSOR MOUNTING LOCATION

The position of the sensor is one of the most important considerations for accurate flow measurement. The same location guidelines apply to Transit Time as most other flow meter technologies.

VERTICAL OR HORIZONTAL PIPE - Vertical pipe runs are acceptable, and the transducers can be mounted in any orientation around the pipe. Downward flow should be avoided in case the pipe becomes partially filled or aerated. On Horizontal pipes and liquids with high concentrations of gas or solids, the sensors should be mounted on the side (1 to 5 o'clock positions) to avoid concentrations of gas at the top of the pipe, or solids at the bottom.

5 D	la ————————————————————————————————————		10 Dia	
FLOW	0 •	0		

1 TO 5 O'CLOCK POSITION ON HORIZONTAL PIPES	
	0
ANY POSITION ACCEPTABLE WITH VERTICAL FLOW	0
	\smile

STRAIGHT RUN REQUIREMENTS – For best results, the transducers must be installed on a straight run of pipe, free of bends, tees, valves, transitions, insertion probes and obstructions of any kind. For most installations, ten straight unobstructed pipe diameters upstream and five diameters downstream of the transducers is the minimum recommended distance for proper operation. Additional considerations are outlined below.

- Do not, if possible, install the transducers downstream from a throttling valve, a mixing tank, the discharge of a positive displacement pump or any other equipment that could possibly aerate the liquid. The best location will be as free as possible from flow disturbances, vibration, sources of heat, noise, or radiated energy.
- Avoid mounting the transducers on a section of pipe with any external scale. Remove all scale, rust, loose paint, etc., from the location prior to mounting the transducers. A sanding block is included with every meter to facilitate proper pipe preparation.
- Do not mount the transducers on a surface aberration (pipe seam, etc.).
- Do not mount transducers from different ultrasonic flow meters on the same pipe.
- Do not run the transducer triaxial cables in common bundles with cables from other instrumentation. You can run these cables through a common conduit ONLY if they originate at the same flow meter.
- Never mount transducers under water.

IMPORTANT NOTE: In some cases, longer straight runs may be necessary where the transducers are placed downstream from devices which cause unusual flow profile disruptions or swirl. For example: modulating valves, or two elbows in close proximity and out of plane.



SEPARATION DISTANCE (Sensor Spacing Distance)

Separation distance is automatically calculated by the TTFM 6.1 based on parameters entered in the Setup menu. Sens Space is parameter where this distance is given, and it is located in the Setup menu. Document this value for the following transducer installation procedure.

2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B TMK-B1 Kit

1. Prep the pipe per instructions on page 29, and mind the installation location requirements on page 32. Clean the location where the sensor is to be mounted on the opposite side of the pipe after we've marked where it will be installed. Picture below shows a very clean ductile iron pipe which did not require much cleaning. The outside paint is very well bonded and did not need to be removed:



2. Install the stainless steel mounting brackets on the pipe. Position them at approximately the correct separation distance. Exact measurement is not required at this time. Tip: Use a 5/16" nut driver to tighten the hose clamps.

Procedure continued on the next page...



2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B Transducers TMK-B1 Kit (Cont.)

3. Use alignment bar to ensure the brackets are parallel. Completion of steps 2 & 3 is shown below.

- 4. Mark the position of the permanent bracket on the pipe. This is the bracket that will not be adjusted, and will be used as the reference for the separation distance and alignment. It is your choice which bracket is permanent. With a marker, mark the bracket position by placing the mark directly in front of the stainless side-rail.






2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B Transducers TMK-B1 Kit (Cont.)

5. Measure the separation distance from the mark you created in step 4, and create a new mark on the pipe at the separation distance. It may be useful to mark your Greyline tape measure (included with every meter) at the separation distance point before marking the pipe. The marked pipe is shown below.



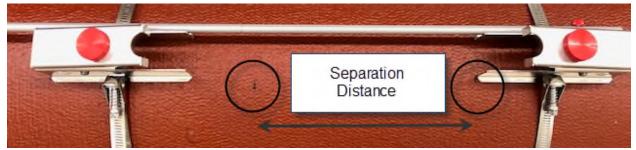

6. Move the non-permanent bracket to position at the mark you created at step 5, and tighten it completely. Apply coupling compound to the transducers, and install them in the brackets.

Tips for installing transducers:

- a. Be sure the red knob on the brackets are loosened completely
- b. Put the transducer into the bracket by ensuring the bottom of the transducer and the couplant does not touch the pipe as you slide it in. (Hover)
- c. With the transducer hovering, tighten the red knob on the bracket until thight. The transducer will be level with the surface of the pipe, and no grease will have smeared off.

(pictures of proper coupling application and finished installation on the next page)



2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B Transducers TMK-B1 Kit (Cont.)

Proper coupling compound application:

Finished installation, ready for cable connection:



7. If you need to make fine adjustments $(\pm 0.25")$ to the spacing at this point, you may do so by loosening the hose clamps slightly, and sliding the brackets while the transducers are installed inside them. Tighten hose clamps when done.



SEPARATION DISTANCE (Sensor Spacing Distance)

Separation distance is automatically calculated by the TTFM 6.1 based on parameters entered in the Setup menu. Sens Space is parameter where this distance is given, and it is located in the Setup menu. Document this value for the following transducer installation procedure.

1 CROSS INSTALLATION OVERVIEW – SE16B Transducers TMK-B1 Kit

To assist with the proper installation of the transducers in a 1 cross installation, we provide a kit with every meter, which consists of the following:

- Sanding block
- Tape measure
- Mylar sleeve
- Duct tape
- Level
- Black Sharpie

Follow along with the 1 cross installation instructions on the following pages for a description of where to use these tools.

1. Prep the pipe per instructions on page 29, and mind the installation location requirements on page 32. Clean the location where the sensor is to be mounted on the opposite side of the pipe after we've marked where it will be installed. The picture below shows a very clean ductile iron pipe which did not require much cleaning.



Page 37



2. Install one of the stainless steel mounting brackets on the pipe. This will be the stationary bracket not being rotated to the opposite side of the pipe. For a horizontal pipe, position the bracket at 3 or 9 o'clock. Hold the level up to the top of the bracket to ensure the angle is correct. For vertical pipes, the bracket can be at any orientation about the pipe. Tip: Use a 5/16" nut driver to tighten the hose clamp. Install the second bracket at approximately the distance specified by the Sens Space value in the Setup menu.




3. Use alignment bar to ensure that the brackets are parallel. Completion of steps 2 and 3 is shown below.





4. Mark the position of the bracket on the pipe. Mark both where the front of the bracket is, as well as the center of the bracket.

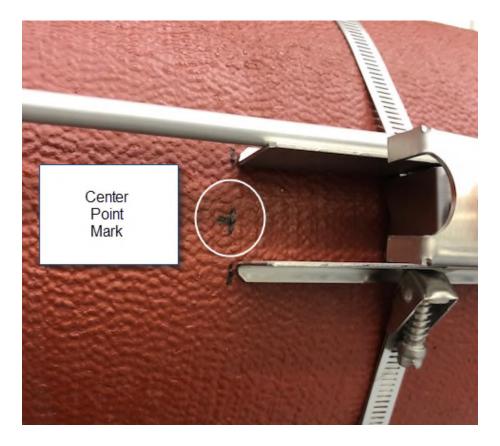

5. Measure the separation distance from the marks you created in step 4, and create new marks on the pipe at the separation distance. It may be useful to mark your Greyline tape measure at the separation distance before holding it up to and marking the pipe.





6. Using the mylar sleeve included with the installation kit, wrap it around the pipe, keep it taut, and with the Sharpie, draw a line anywhere the sleeve overlaps:




7. Lay the mylar sleeve flat, use duct tape to help hold it flat if you need to, and use the tape measure to measure half way between the two marks created when you wrapped the mylar around the pipe:





8. Position the marked mylar back on the pipe, with the overlap marks on the center line of the transducer bracket that will be rotated to the other side of the pipe. Be sure the mylar is parallel with the face of the transducer. Use duct tape to hold the mylar together and to the pipe. While the mylar is in this position, mark the opposite side of the pipe where the mylar is marked from step 7:

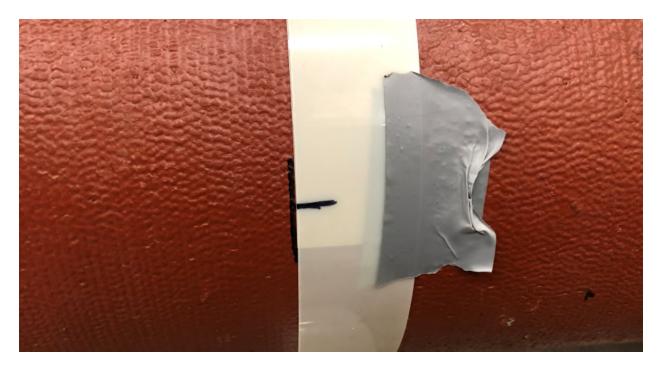





9. Sand the pipe at this position if it needs to be prepped because of scale or rust. After prepped, move the bracket to this 1 cross mark, and tighten it in place. Apply coupling compound to the transducers and place them in the brackets:

Tips for installing transducers:

- a. Be sure the red knob on the brackets are loosened completely.
- b. Put the transducer into the bracket by ensuring the bottom of the transducer and the couplant does not touch the pipe as you slide it in (hover).
- c. With the transducer hovering, tighten the red knob on the bracket until tight. The transducer will be level with the surface of the pipe, and no grease will have smeared off from inserting the transducer in the bracket.

Proper coupling compound application:







Finished installation:

10. If you need to make fine adjustments $(\pm 0.25")$ to the spacing at this point, you may do so by loosening the hose clamps slightly, and sliding the brackets while the transducers are installed inside them. Tighten the hose clamps when done.



SEPARATION DISTANCE (Sensor Spacing Distance)

Separation distance is automatically calculated by the TTFM 6.1 based on parameters entered in the Setup menu. Sens Space is parameter where this distance is given, and it is located in the Setup menu. Document this value for the following transducer installation procedure.


2 OR 4 CROSS INSTALLATION OVERVIEW – SE16B Transducers TMK-B21 or TMK-B22 Kit

1. Prep the pipe per instructions on page 29, and mind the installation location requirements on page 32. Clean the location where the sensor is to be mounted on the opposite side of the pipe after we've marked where it will be installed. Picture below shows a very clean ductile iron pipe which did not require much cleaning. The outside paint is very well bonded and did not need to be removed:






2. Install the spacer bar onto the right bracket as shown below:

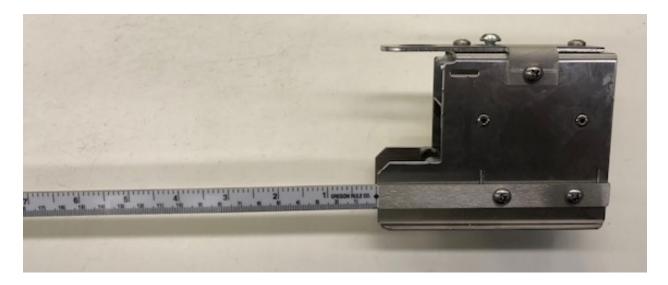

3. Insert the spacer bar into the left bracket, and position the bracket at the separation distance referenced earlier. Tighten the spacer bar clamp at this position:

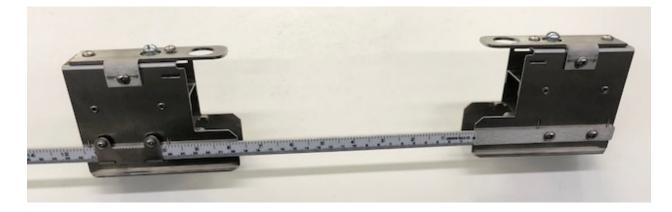



4. Place the bracket assembly on the pipe, tighten it in place with the two hose clamps:



5. Apply coupling compound to the transducers, and install them in the brackets.

Tips for installing transducers:

- a. Be sure the tightening Philips screw on the top of the bracket is loosened completely.
- b. Put the transducer into the bracket by ensuring the bottom of the transducer and the couplant does not touch the pipe as you slide it in. (Hover)
- c. Tighten the Phillips screws on the bracket until tight. The transducer will be level with the surface of the pipe, and no grease will have smeared off.

(pictures of proper coupling application and finished installation on the next page)



Proper coupling compound application:

Finished installation, ready for cable and conduit connection:



6. If you need to make fine adjustments $(\pm 0.25")$ to the spacing at this point, you may do so by loosening the hose clamps slightly, and sliding the brackets while the transducers are installed inside them. Tighten hose clamps when done.



SEPARATION DISTANCE (Sensor Spacing Distance)

Separation distance is automatically calculated by the TTFM 6.1 based on parameters entered in the Setup menu. Sens Space is parameter where this distance is given, and it is located in the Setup menu. Document this value for the following transducer installation procedure.

1 CROSS INSTALLATION OVERVIEW – SE16B Transducers TMK-B21 or TMK-B22 Kit

To assist with the proper installation of the transducers in a 1 cross installation, we provide a kit with every meter, which consists of the following:

- Sanding block
- Tape measure
- Mylar sleeve
- Duct tape
- Level
- Black Sharpie

Follow along with the 1 cross installation instructions on the following pages for a description of where to use these tools.

1. Prep the pipe per instructions on page 29, and mind the installation location requirements on page 32. Clean the location where the sensor is to be mounted on the opposite side of the pipe after we've marked where it will be installed. The picture below shows a very clean ductile iron pipe which did not require much cleaning.





2. Install the spacer bar onto the right bracket as shown below:



3. Insert the spacer bar into the left bracket, and position the bracket at the separation distance referenced earlier. Tighten the spacer bar clamp at this position:





4. Place the bracket assembly on the pipe, tighten it in place with the two hose clamps. For a horizontal pipe, position the bracket at 3 or 9 o'clock. Hold the level up to the top of the bracket to ensure the angle is correct. For vertical pipes, the bracket can be at any orientation about the pipe. Tip: Use a 5/16" nut driver to tighten the hose clamp.



5. Mark the position of the center line of the bracket which is to be moved to the opposite side of the pipe. It is up to you to determine which bracket is easier to move from the current position:





6. Using the mylar sleeve included with the installation kit, wrap it around the pipe, keep it taut, and with the Sharpie, draw a line anywhere the sleeve overlaps:



7. Lay the mylar sleeve flat, and use the tape measure to measure half way between the two marks created when you wrapped the mylar around the pipe:





8. Position the marked mylar back on the pipe, with the overlap marks on the center line of the transducer bracket that will be rotated to the other side of the pipe. Be sure the mylar is parallel with the face of the transducer. Use duct tape to hold the mylar together and to the pipe. While the mylar is in this position, mark the opposite side of the pipe where the mylar is marked from step 7:








9. Sand the pipe at this position if it needs to be prepped because of scale or rust. After prepped, move the bracket to this 1 cross mark, and tighten it in place. Apply coupling compound to the transducers and place them in the brackets:

View from front of pipe:



View from back of pipe:

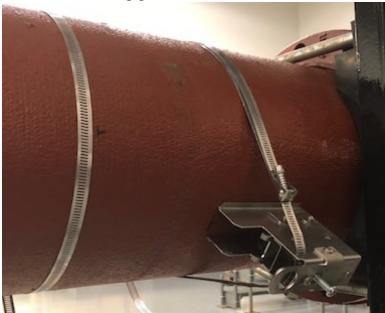


Tips for installing transducers:

- a. Be sure the tightening screws on the brackets are loosened completely.
- b. Put the transducer into the bracket by ensuring the bottom of the transducer and the couplant does not touch the pipe as you slide it in (hover).



c. With the transducer hovering, tighten the screws on the bracket until tight. The transducer will be level with the surface of the pipe, and no grease will have smeared off from inserting the transducer in the bracket.

Proper coupling compound application:

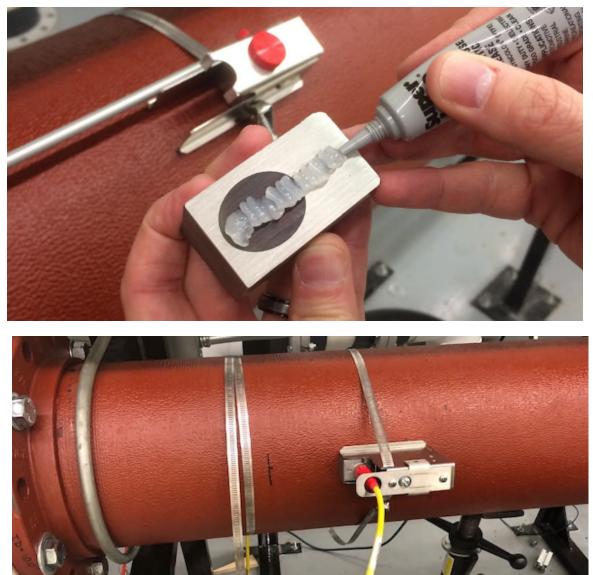

Finished installation:

10. If you need to make fine adjustments (± 0.25 ") to the spacing at this point, you may do so by loosening the hose clamps slightly, and sliding the brackets while the transducers are installed inside them. Tighten the hose clamps when done.




SEPARATION DISTANCE (Sensor Spacing Distance)

Separation distance is automatically calculated by the TTFM 6.1 based on parameters entered in the Setup menu. Sens Space is parameter where this distance is given, and it is located in the Setup menu. Document this value for the following transducer installation procedure.

2 or 4 CROSS INSTALLATION OVERVIEW – SE16A Transducers TMK-A1 Kit

- 1. Prep the pipe per instructions on page 30, and mind the installation location requirements on page 32. Clean the location where the mounting track is to be installed.
- 2. Install the stainless steel mounting track on the pipe. Place the tightening brackets near the center, as the transducers are inserted from the outside of them.

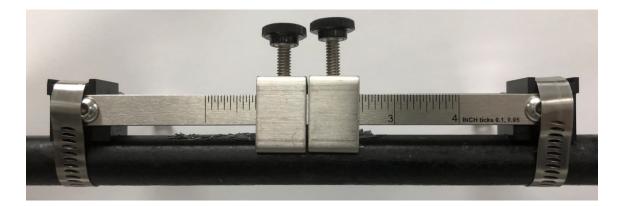




3. Apply a small amount of coupling compound on the first transducer, and place this transducer in the "reference" position. This is the position where the face of the transducer aligns with the 0 inch or 0 mm mark on the built-in ruler. Tighten this transducer down using the built-in tightening bracket. Do not over-tighten the screw.








4. Apply a small amount of coupling compound on the second transducer, and place this transducer at the separation distance provided in the Setup menu of the TTFM. Tighten this transducer down using the built-in tightening bracket. Do not over-tighten the screw.

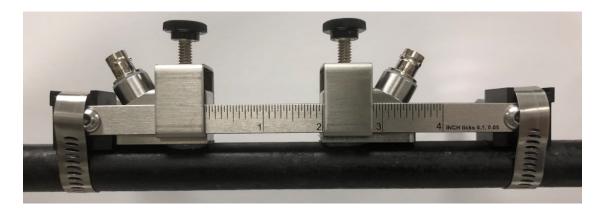

5. If you need to make fine adjustments $(\pm 0.1^{"})$ to the spacing at this point, you may do so by loosening the tightening screw slightly, sliding the second transducer, then re-tightening it.



TTFM 6.1 Transit Time Flow Meter

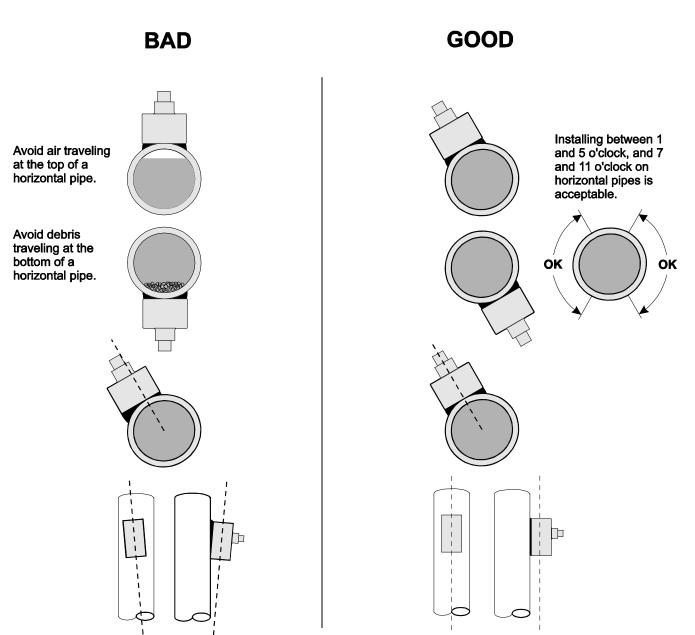

SENSOR MOUNTING/COUPLING RECOMMENDATIONS



ENCLOSURE INSTALLATION

Locate the enclosure within 25 ft (7.6 m) of the sensors (up to 100 ft - 30 m optional). The enclosure can be wall mounted with the four mounting screws (included) or panel mounted with Option PM Panel Mount kit from Greyline Instruments.

Avoid mounting the enclosure in direct sunlight to protect the electronics from damage due to overheating and condensate. In high humidity atmospheres, or where temperatures fall below freezing, Option TH Enclosure Heater and Thermostat is recommended. **IMPORTANT**: Seal conduit entries to prevent moisture from entering enclosure.


NEMA4X (IP66) WITH CLEAR COVER


1. Open hinged enclosure cover.

2. Insert #12 screws (supplied) through the four enclosure mounting holes to secure the enclosure to the wall or mounting stand.

Additional conduit holes can be cut in the bottom of the enclosure when required. Use a hole saw or Greenlee-type hole cutter to cut the required holes.

IMPORTANT: DO NOT make conduit/wiring entries into the top or sides of the enclosure.





Note: This non-metallic enclosure does not automatically provide grounding between conduit connections. Grounding must be provided as part of the installation. Ground in accordance with the requirements of the National Electrical Code. System grounding is provided by connecting grounding wires from all conduit entries to the steel mounting plate or another point which provides continuity.

CLEANING

Cleaning is not required as a part of normal maintenance.



FIELD TROUBLESHOOTING

Possible Causes:

Corrective Action:

METER READING WHEN THERE IS NO FLOW?

Erratic measurement (set damping to 0% to check) due to electrical noise or poor signal quality.	 Set Calibration/Damping to 0% with zero flow use Setup / Tare function. Ensure all Flowmeter wiring is in METAL conduit and sensor shield is properly connected to Ground. Ensure correct power input Ground connection (<1 ohm resistance). Ensure 4-20mA Shield connected to Instrument Ground stud. Adjust Calibration/MinFlow setting. Contact Greyline for further assistance.
Variable Speed Drive interference	 Follow Drive manufacturers wiring and Grounding instructions Relocate Flowmeter electronics, Sensor and wiring away from VSD

METER READING LOWER THAN EXPECTED?

Calibration Error	• Review calibration menu. Pipe dimensions and fluid selection/fluid velocity.
Lower flow rate than expected	• Investigate pump/valves. Compare velocity with alternate instrument.
Erratic measurement (set damping to 0% to check) due to electrical noise or poor signal quality.	 Ensure all Flowmeter wiring is in METAL conduit and sensor shield is properly grounded. Ensure correct power input Ground connection (<1 ohm resistance). Ensure 4-20mA Shield connected to Instrument Ground stud. Contact Greyline for further assistance.

NO ECHO INDICATION Icon: No Echo

Improper Installation	• Check Setup menu to ensure pipe material, size, thickness, liner type, thickness, fluid type, and fluid temperature and configured properly. Check transducer mounting method and spacing matches Setup menu values.
Sensors not mounted to Pipe or mounted improperly	• Apply coupling compound and mount sensors to pipe with proper sensor spacing.



Possible Causes:	Corrective Action:						
NO ECHO INDICATION Icon: No Ec	ho (cont.)						
Empty pipe or partially filled	• Pipe must be fluid filled and acoustically transparent in order to obtain echoes.						
Coupling compound washed out, or sensor loose on pipe.	 Remount sensor Use Super Lube® Silicone Compound 						
SENSOR CONNECTIONS							
OPEN/SHORT SENSOR ICON	 No sensors attached Short in transducer, or in triax transducer cable. Follow Sensor Connections steps 						
Sensor Connections	 Check sensor connections at TTFM and at sensor junction box. Note: Refer to Sensor Cable Resistance Test to test final connections. 						
METER READING HIGHER THAN E	XPECTED?						
Calibration Error	• Review calibration menu. Pipe dimensions and fluid selection/fluid velocity.						
Higher flow rate than expected	• Investigate pump/valves. Compare velocity with alternate instrument.						
Erratic measurement (set damping to 0% to check) due to electrical noise or poor signal quality.	 Ensure all Flowmeter wiring is in METAL conduit and sensor shield is properly grounded. Ensure correct power input Ground connection (<1 ohm resistance). Ensure 4-20mA Shield connected to Instrument Ground stud. Contact Greyline for further assistance. 						
High viscosity fluid	• Laminar flow profile due to high viscosity fluid requires an adjustment to Cal Const.						




SENSOR CABLE & TRANSDUCER RESISTANCE TEST

Unplug the green sensor terminal from the Transit Time board with the sensor wires still connected and the BNC end of the cable is connected to the transducer. With a multimeter, perform resistance checks for each set of wires. One single loose terminal may cause false readings.

Test across shield and core of each wire: TDR1 and TDR2. Resistance should be around 10K ohms for any cable length. High readings indicate an open circuit and low readings indicate a short or partial short in the sensor cable connections or transducer.

Note: The TTFM 6.1 will automatically detect connectivity to the sensors. Confirm that TTFM 6.1 indicates "Sensor Good" in the messages menu if your resistance measured is approximately 10K Ohms.

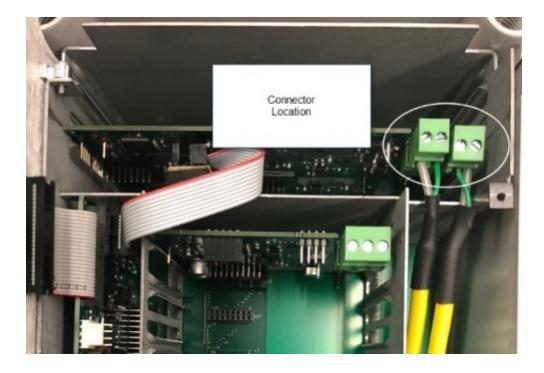





COMMON QUESTIONS AND ANSWERS

The pipe vibrates. Will it affect the flow meter?

Common vibration frequencies are far lower than the sonic frequencies used by the Greyline flow meter, and will not normally affect accuracy or performance. However, applications where very weak Transit Time signal is present (when sensitivity is adjusted to maximum and signal strength is low), accuracy may be affected by pipe vibration, or the flow meter may show readings under no-flow conditions. Attempt to relocate the sensor on a pipe section where vibration is reduced, or arrange pipe mounting brackets to reduce vibration at the sensor mounting location.

The flow meter must be installed in a high noise environment. Will this affect operation?

Greyline flow meters are designed to discriminate between environmental noise and the Transit Time signal. High noise environments may affect the flow meter's performance where low signal strength and/or low flow velocities are being measured. Relocate the sensor in a quieter environment if possible.

Will pipe corrosion affect accuracy of the flow meter?

Yes. Rust, loose paint etc. must be removed from the outside of the pipe to provide a clean mounting position when installing a Transit Time sensor. Severe corrosion/oxidation on the inside of the pipe may prevent the Transit Time signal from penetrating into the flow. If the pipe cannot be cleaned, a spool piece (PVC recommended) should be installed for sensor mounting.

What effect do pipe liners have on the flow meter?

The air gap between loose insertion liners and the pipe wall prevent the Transit Time signal from entering the flow. Better results can be expected with bonded liners such as cement, epoxy or tar, however an on site test is recommended to determine if the application is suitable for a Transit Time flow meter.

Why is Transit Time recommended for clean liquids?

The Transit Time sensor transmits sound across the flow stream in order to measure the time it takes to arrive at the other sensor, and therefore requires a fluid medium that is relatively transparent to the acoustic signal. The Transit Time system will not function when there is high volume of solids or aeration. As a guideline, Greyline Transit Time flow meters are recommended for clean liquids with solids or bubbles content less than 2% by volume.

Can the sensor be submerged in water?

Yes, for short periods of time or by accident, but it is not recommended for continuous operation. The sensor is constructed to withstand submersion to 10 psi (0.7 Bar) without damage provided the protective rubber boot is filled with Super Lube®.



What is the purpose of the Signal Strength Display?

The primary function of the signal strength display is to assist as a feedback when mounting sensors. Signal Strength can also be a useful diagnostics tool when troubleshooting problems with an installation. A signal strength less than 100% may indicate a problem with the installation or other issues such as a mis-programmed pipe size, pipe material, fluid type or temperature, or wrong transducer spacing. A signal strength less than 100% may also simply indicate a lot of aeration, or deteriorated pipe. Consideration should be made to use a 1 cross installation in such a case.

Can I change the length of the sensor cable?

Yes. The Greyline Transit Time design allow cable lengths up to 100 ft (30 m) or extension up to 250 ft with extra cable and JB2X optional junction box. Replacement cable of different length may be installed in rigid or flexible conduit for mechanical protection. Use only Greyline shielded triaxial cable.

Does the TTFM 6.1 require periodic recalibration?

TTFM 6.1 calibration does not drift over time. The solid state sensor has no moving parts to wear and affect calibration. All Greyline timing/counting circuits use crystal-controlled frequency references to eliminate any drift in the processing circuitry.

ISO 9000 or similar quality management systems may require periodic and verifiable recalibration of flow meters. TTFM 6.1 Flow Meters may be returned to Greyline for factory calibration and issue of a new NIST traceable certificate. Refer to the 'Product Return Procedure' section of this manual for return instructions.



TTFM 6.1 Transit Time Flow Meter

APPLICATIONS HOTLINE

For applications assistance, advice or information on any Greyline Instrument contact your Sales Representative, write to Greyline or phone the Applications Hotline below:

United States:	Tel: 315-788-9500	Fax: 315-764-0419
Canada:	Tel: 613-938-8956	Fax: 613-938-4857
Toll Free:	888-473-9546	
Email:	info@greyline.com	
Web Site:	www.greyline.com	

Greyline Instruments Inc.

USACanada11451 Belcher Road South16456 Sixsmith DriveLargo, FL 33773Long Sault, Ont. K0C 1P0

PRODUCT RETURN PROCEDURE

Instruments may be returned to Greyline for service or warranty repair.

1 Obtain an RMA Number from Greyline -

Before shipping a product to the factory please contact Greyline by telephone, fax or email to obtain an RMA number (Returned Merchandise Authorization). This ensures fast service and correct billing or credit.

When you contact Greyline please have the following information available:

- 1. Model number / Software Version
- 2. Serial number
- 3. Date of Purchase
- 4. Reason for return (description of fault or modification required)
- 5. Your name, company name, address and phone number

2 Clean the Sensor/Product -

Important: unclean products will not be serviced and will be returned to the sender at their expense.

- 1. Rinse sensor and cable to remove debris.
- 2. If the sensor has been exposed to sewage, immerse both sensor and cable in a solution of 1 part household bleach (Javex, Clorox etc.) to 20 parts water for 5 minutes. Important: do not immerse open end of sensor cable.
- 3. Dry with paper towels and pack sensor and cable in a sealed plastic bag.
- 4. Wipe the outside of the enclosure to remove dirt or deposits.
- 5. Return to Greyline for service.



LIMITED WARRANTY

Greyline Instruments warrants, to the original purchaser, its products to be free from defects in material and workmanship for a period of one year from date of invoice. Greyline will replace or repair, free of charge, any Greyline product if it has been proven to be defective within the warranty period. This warranty does not cover any expenses incurred in the removal and re-installation of the product.

If a product manufactured by Greyline should prove defective within the first year, return it freight prepaid to Greyline Instruments along with a copy of your invoice.

This warranty does not cover damages due to improper installation or handling, acts of nature, or unauthorized service. Modifications to or tampering with any part shall void this warranty. This warranty does not cover any equipment used in connection with the product or consequential damages due to a defect in the product.

All implied warranties are limited to the duration of this warranty. This is the complete warranty by Greyline and no other warranty is valid against Greyline. Some states do not allow limitations on how long an implied warranty lasts or limitation of incidental or consequential damages, so the above limitations or exclusions may not apply to you.


This warranty gives you specific legal rights, and you may also have other rights which vary from state to state.

Greyline Instruments Inc.



ENCLOSURE HEATER AND THERMOSTAT - Option TH

Instruments can be factory-equipped with an Enclosure Heater and Thermostat or the module can be customer-installed. The Thermostat is factory set to turn ON at 40°F (4.5° C) and OFF at 60°F (15.5° C). Power consumption is 15 Watts.

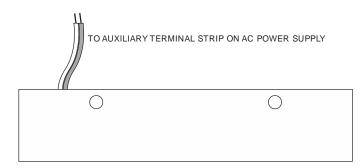

ENCLOSURE SUNSCREEN - Option SCR


Do not mount instrument electronics in direct sunlight. Overheating will reduce the life of electronic components and condensate may form during the heat/cool cycles and cause electrical shorts.

Note:

Exposure to direct sunlight can cause overheating and moisture condensation which will reduce the operating life of electronics.

Protect Instruments from direct sunlight with this iridite finished aluminum sun screen (Greyline Option SCR).

Seal conduit entries with caulking compound to further reduce moisture condensation.

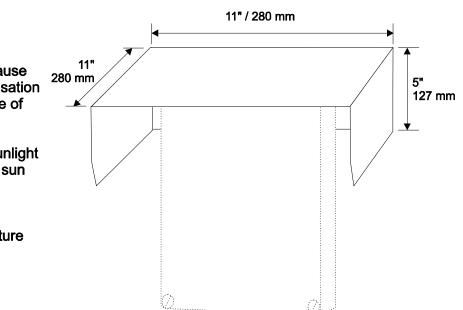




TTFM 6.1 Transit Time Flow Meter

POWER INPUT OPTION 9-32VDC

TTFM 6.1 Flow Meters may be ordered factory-configured for 9-32VDC power input, or a 9-32VDC Power Input card can be installed in the place of the 100-240VAC card in the field.

CONNECTIONS:

POWER INPUT: Connect 9-32VDC to the + and - terminals. The Power Input GND terminal must be connected to the nearest Ground pole. A 1 amp fuse in line is recommended.

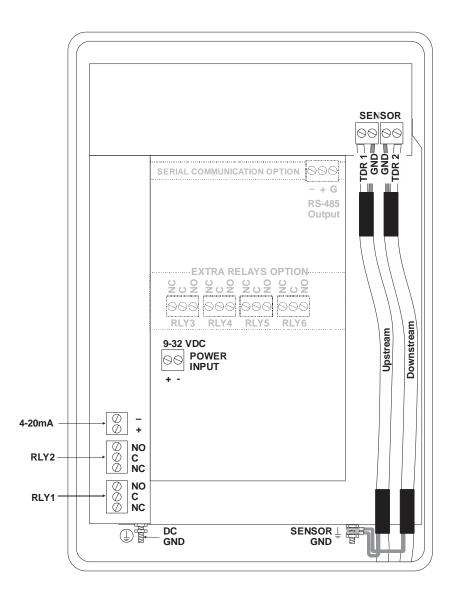



← 7.4" / 188 mm →

SPECIFICATIONS

Flow Rate Range:	±0.07 to 40 ft/sec (±0.02		←5.12" / 130 mm→
Dine Cire	to 12 m/sec)	p	
Pipe Size:	¹ / ₂ " to 48" (15 to 1200		
Accuracy:	mm) ±1% of flow rate from 1.5		
Accuracy.	to 40 ft/sec, ± 0.015 ft/sec		10.94" / 278 mm - 10" / 254 mm -
	below 1.5 ft/sec.		78
	Repeatability and		2541
	Linearity: ±0.25%		"44"
Displays:	White, backlit matrix -		- Γ Γ
Displays:	displays flow rate,	TTFM 6.1 Greyline	
	totalizer, relay states,	Ultrasoric Flow Motor	
	operating mode and		
	calibration menu		[]===========================
Calibration:	built-in 5-key calibrator	CONDUIT ENTRY	SIDE VIEW
	with English, French or	LOCATION	
	Spanish language selection	1	
Power Input:	100-240VAC, 50/60Hz, 10\		
	Optional 9-32VDC, 10 Wat	ts Maximum	
Output:	Isolated 4-20mA (1000 ohn	n load max.). Can be cl	hanged to 0-5VDC in
	programming		
Data Logger:	128MB Data Storage, 26 m	illion data points	
Control Relays:	Qty 2, rated 5 amp 240VAC	C SPDT, programmable	e flow alarm and/or
	proportional pulse		
Enclosure:	Watertight, dust tight NEMA	A4X (IP 66) polycarbon	ate with a clear
	shatter-proof face		
Environmental Conditions:	Relative humidity up to 80%		
	maximum 5000 m altitude,		tallation Category II.
Electrical Surge Protection:	Sensor, 4-20mA output and	AC power input	
Approximate Shipping Weight:	12 lbs (5.5 kg)		


SE16B Transit Time Sensor

Pipe Diameter: Operating Temperature: Exposed Materials: Operating Frequency: Sensor Cable: Submersion Rating:	2" to 48" (50 to 1200 mm) -40° to 300°F (-40° to 150°C) 316SS 1.28 MHz 25 ft (7.6 m) Optional 50 ft (15 m) or 100 ft (30 m) available, extendable up to 500 ft (150 m) with JB2X optional junction box. Withstands accidental submersion pressure up to 10 psi (0.7 Bar) when installed with Super Lube® in sealing rubber boot.
	56 mm 2.2" 32 mm 1.25" SIDE VIEW 54 mm / 2.1" SIDE VIEW SE16B SENSOR DIMENSIONS SUBE VIEW SIDE VIEW SE16B SENSOR DIMENSIONS SE16B SENSOR SIDE VIEW SIDE VIEW SIDE VIEW SE16B SENSOR SIDE VIEW SIDE VIEW SE16B SENSOR SIDE VIEW SIDE VIEW




SE16A Transit Time Sensor

Pipe Diameter:	0.5" To 4" (15 to 100 mm)
Operating Temperature:	-40° to 300°F (-40° to 150°C)
Exposed Materials:	316SS
Operating Frequency:	2.56 MHz
Sensor Cable:	25 ft (7.6 m)
	Optional 50 ft (15 m) or 100 ft (30 m) available, extendable up to 500 ft (150 m) with JB2X optional junction box.
Submersion Rating:	Withstands accidental submersion pressure up to 10 psi (0.7 Bar)

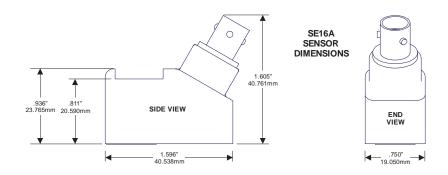

SE16A Track Mount Dimensions

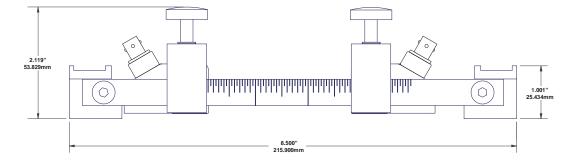

TTFM 6.1 Transit Time Flow Meter



APPENDIX A - CONVERSION TABLE

CONVERSION GUIDE									
FROM	то	MULTIPLY BY							
US GALLONS	CUBIC FEET	0.1337							
US GALLONS	IMPERIAL GALS	0.8327							
US GALLONS	LITRES	3.785							
US GALLONS	CUBIC METERS	0.003785							
LITRES/SEC	GPM	15.85							
LITRES	CUBIC METERS	0.001							
BARRELS (bbl)	US GALLONS	42							
BARRELS (bbl)	IMPERIAL GALS	34.9726							
BARRELS (bbl)	LITRES	158.9886							
INCHES	MM	25.4							
DEGREES F	DEGREES C	(°F-32) x 0.556							
POUNDS	KILOGRAMS	0.453							
PSI	BAR	0.0676							
FOOT ²	METER ²	0.0929							

Note: BARRELS (bbl) are U.S. oil barrels.



PIPE CHARTS

Note: Not all pipe types allowed in programming have charts below. Pipe dimensions will need to be acquired from pipe markings or the pipe manufacturer in such cases.

Pipe	Pipe	Schedule	Standard	Extra	Heavy	Dbl. Extr	a Heavy	Sched	ule 10	Schedule 20		Schedule 30		Schedule 40		Schedule 80	
Size	O.D.	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL
1/2 3/4 1 1 1/4 1 1/2	0.840 1.050 1.315 1.660 1.900	0.622 0.824 1.049 1.380 1.900	0.109 0.113 0.133 0.140 0.145											0.622 0.824 1.049 1.380 1.900	0.109 0.113 0.133 0.140 0.145	0.546 0.742 0.957 1.278 1.500	0.147 0.154 0.175 0.191 0.200
2	2.375	2.067	.154	1.939	.218	1.503	.436							2.067	.154	1.939	0.218
2 ¹ / ₂ 3	2.875 3.500	2.469 3.068	.203 .216	2.323 2.900	.276 .300	1.771 2.300	.552 .600							2.469 3.068	.203 .216	2.323 2.900	0.276 0.300
3 ¹ / ₂	4.000	3.548	.226	3.364	.318	2.728	.636							3.548	.226	3.364	0.318
4	4.500	4.026	.237	3.826	.337	3.152	.674							4.026	.237	3.826	0.337
5	5.563	5.047	.258	4.813	.375	4.063	.750							5.047	.258	4.813	0.375
6	6.625	6.065	.280	5.761	.432	4.897	.864							6.065	.280	5.761	0.432
8	8.625	7.981	.322	7.625	.500	6.875	.875			8.125	.250	8.071	.277	7.981	.322	7.625	0.500
10	10.750	10.020	.365	9.750	.500	8.750	1.000			10.250	.250	10.136	.307	10.020	.365	9.564	0.593
12	12.750	12.000	.375	11.750	.500	10.750	1.000			12.250	.250	12.090	.330	11.938	.406	11.376	0.687
14	14.000	13.250	.375	13.000	.500			13.500		13.376	.312	13.250	.375	13.124	.438	12.500	0.750
16	16.000	15.250	.375	15.000	.500			15.500		15.376	.312	15.250	.375	15.000	.500	14.314	0.843
18	18.000	17.250	.375	17.000	.500			17.500		17.376	.312	17.124	.438	16.876	.562	16.126	0.937
20	20.000	19.250	.375	19.000	.500 .500			19.500		19.250	.375	19.000	.500	18.814	.593	17.938	1.031
22 24	22.000 24.000	21.250	.375	21.000 23.000				21.500 23.500		21.250 23.250	.375 .375	21.000 22.876	.500	22.626	.687	04 564	1 010
		23.250	.375		.500						.375	22.870	.562	22.020	.007	21.564	1.218
26 28	26.000 28.000	25.250 27.250	.375 .375	25.000 27.000	.500 .500			25.376 27.376		25.000 27.000	.500 .500	26.750	.625				
28 30	28.000 30.000	27.250 29.250	.375	29.000	.500 .500			29.376		27.000	.500	28.750	.625 .625				
32	32.000	31.250	.375	31.000	.500			31.376		31.000	.500	30.750	.625				
34	34.000	33.250	.375	33.000	.500			33.376		33.000	.500	32.750	.625				
36	36.000	35.250	.375	35.000	.500			35.376		35.000	.500	34.750	.625				
42	42.000	41.250	.375	41.000	.500					41.000	.500	40.750	.625				

Carbon Steel & PVC Pipe

Ductile Iron Pipe – Standard Classes

Size	OUTSIDE	Class		CEMENT	LINING																										
INCH	DIA.																													**STD	**DOUBLE
	INCH	WALL	I.D.	THICKNESS	THICKNESS																										
3	3.96			0.25	3.46	0.28	3.40	0.31	3.34	0.34	3.28	0.37	3.22	0.41	3.14	.125	.250														
4	4.80			0.26	4.28	0.29	4.22	0.32	4.16	0.35	4.10	0.38	4.04	0.44	3.93																
6	6.90	0.25	6.40	0.28	6.34	0.31	6.28	0.34	6.22	0.37	6.16	0.40	6.10	0.43	6.04																
8	9.05	0.27	8.51	0.30	8.45	0.33	8.39	0.36	8.33	0.39	8.27	0.42	8.21	0.45	8.15																
10	11.10	0.39	10.32	0.32	10.46	0.35	10.40	0.38	10.34	0.41	10.28	0.44	10.22	0.47	10.16																
12	13.20	0.31	12.58	0.34	12.52	0.37	12.46	0.40	12.40	0.43	12.34	0.46	12.28	0.49	12.22																
14	15.30	0.33	14.64	0.36	14.58	0.39	14.52	0.42	14.46	0.45	14.40	0.48	14.34	0.51	14.28																
16	17.40	0.34	16.72	0.37	16.66	0.40	16.60	0.43	16.54	0.46	16.48	0.49	16.42	0.52	16.36																
18	19.50	0.35	18.80	0.38	18.74	0.41	18.68	0.44	18.62	0.47	18.56	0.50	18.50	0.53	18.44	.1875	.375														
20	21.60	0.36	20.88	0.39	20.82	0.42	20.76	0.45	20.70	0.48	20.64	0.51	20.58	0.54	20.52																
24	25.80	0.38	25.04	0.41	24.98	0.44	24.92	0.47	24.86	0.50	24.80	0.53	24.74	0.56	24.68																
30	32.00	0.39	31.22	0.43	31.14	0.47	31.06	0.51	30.98	0.55	30.90	0.59	30.82	0.63	30.74																
36	38.30	0.43	37.44	0.48	37.34	0.62	37.06	0.58	37.14	0.63	37.04	0.68	36.94	0.73	36.84																
42	44.50	0.47	43.56	0.53	43.44	0.59	43.32	0.65	43.20	0.71	43.08	0.77	42.96	0.83	42.84	.250	.500														
48	50.80	0.51	49.78	0.58	49.64	0.65	49.50	0.72	49.36	0.79	49.22	0.86	49.08	0.93	48.94																
54	57.10	0.57	55.96	0.65	55.80	0.73	55.64	0.81	55.48	0.89	55.32	0.97	55.16	1.05	55.00																

**REDUCE I.D. BY DIMENSION SHOWN



Schedule 80 S

Stainless Steel, Hastelloy "C" & Titanium Pipe Pipe Pipe Schedule 5 S (a) Schedule 10 S (a) Schedule 40 S Size O.D. I.D. WALL I.D. WALL I.D. WALL

Size	O.D.	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL
1/2 3/4 1 1 1/4 1 1/2	0.840 1.050 1.315 1.660 1.900	0.710 0.920 1.185 1.530 1.770	0.065 0.065 0.065 0.065 0.065	0.674 0.884 1.097 1.442 1.682	0.083 0.083 0.109 0.109 0.109	0.622 0.824 1.049 1.380 1.900	0.109 0.113 0.133 0.140 0.145	0.546 0.742 0.957 1.278 1.500	0.147 0.154 0.175 0.191 0.200
2	2.375	2.245	.065	2.157	.109	2.067	.154	1.939	.218
2 ¹ / ₂	2.875	2.709	.083	2.635	.120	2.469	.203	2.323	.276
3	3.500	3.334	.083	3.260	.120	3.068	.216	2.900	.300
3 ¹ / ₂	4.000	3.834	.083	3.760	.120	3.548	.226	3.364	.318
4	4.500	4.334	.083	4.260	.120	4.026	.237	3.826	.337
5	5.563	5.345	.109	5.295	.134	5.047	.258	4.813	.375
6	6.625	6.407	.109	6.357	.134	6.065	.280	5.761	.432
8	8.625	8.407	.109	8.329	.148	7.981	.322	7.625	.500
10	10.750	10.482	.134	10.420	.165	10.020	.365	9.750	.500
12	12.750	12.438	.156	12.390	.180	12.000	.375	11.750	.500
14	14.000	13.688	.156	13.624	.188				
16	16.000	15.670	.165	15.624	.188				
18	18.000	17.670	.165	17.624	.188				
20	20.000	19.634	.188	19.564	.218				
22	22.000	21.624	.188	21.564	.218				
24	24.000	23.563	.218	23.500	.250				

Pipe	Pipe	Sched	ule 60	Sched	lule 80	Sched	ule 100	Sched	ule 120	Sched	ule 140	Sched	ule 160
Size	O.D.	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL
2	2.375			1.939	.218							1.689	.343
2 ¹ / ₂	2.875			2.323	.276							2.125	.375
3	3.500			2.900	.300							2.624	.438
3 ¹ / ₂	4.000			3.364	.318								
4	4.500			3.826	.337			3.624	.438			3.438	.531
5	5.563			4.813	.375			4.563	.500			4.313	.625
6	6.625			5.761	.432			5.501	.562			5.189	.718
8	8.625	7.813	.406	7.625	.500	7.439	.593	7.189	.718	7.001	.812	6.813	.906
10	10.750	9.750	.500	9.564	.593	9.314	.718	9.064	.843	8.750	1.000	8.500	1.125
12	12.750	11.626	.562	11.376	.687	11.064	.843	10.750	1.000	10.500	1.125	10.126	1.312
14	14.000	12.814	.593	12.500	.750	12.126	.937	11.814	1.093	11.500	1.250	11.188	1.406
16	16.000	14.688	.656	14.314	.843	13.938	1.031	13.564	1.218	13.124	1.438	12.814	1.593
18	18.000	16.500	.750	16.126	.937	15.688	1.156	15.250	1.375	14.876	1.562	14.438	1.781
20	20.000	18.376	.812	17.938	1.031	17.438	1.281	17.000	1.500	16.500	1.750	16.064	1.968
22	22.000	20.250	.875	19.750	1.125	19.250	1.375	18.750	1.625	18.250	1.875	17.750	2.125



Cast Iron Pipe - ASA Standard

Pipe	Pipe	Class	s 50	Class	s 100	Class	150	Clas	s 200	Class	s 250	Class 300		Class 350	
Size	O.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.	WALL	I.D.
3	3.96	0.32	3.32	0.32	3.32	0.32	3.32	0.32	3.32	0.32	3.32	0.32	3.32	0.32	3.32
4	4.80	0.35	4.10	0.35	4.10	0.35	4.10	0.35	4.10	0.35	4.10	0.35	4.10	0.35	4.10
6	6.90	0.38	6.14	0.38	6.14	0.38	6.14	0.38	6.14	0.38	6.14	0.38	6.14	0.38	6.14
8	9.05	0.41	8.23	0.41	8.23	0.41	8.23	0.41	8.23	0.41	8.23	0.41	8.23	0.41	8.23
10	11.10	0.44	10.22	0.44	10.22	0.44	10.22	0.44	10.22	0.44	10.22	0.48	10.14	0.52	10.06
12	13.20	0.48	12.24	0.48	12.24	0.48	12.24	0.48	12.24	0.52	12.16	0.52	12.16	0.56	12.08
14	15.30	0.48	14.34	0.51	14.28	0.51	14.28	0.55	14.20	0.59	14.12	0.59	14.12	0.64	14.02
16	17.40	0.54	16.32	0.54	16.32	0.54	16.32	0.58	16.24	0.63	16.14	0.68	16.04	0.68	16.04
18	19.50	0.54	18.42	0.58	18.34	0.58	18.34	0.63	18.24	0.68	18.14	0.73	18.04	0.79	17.92
20	21.60	0.57	20.46	0.62	20.36	0.62	20.36	0.67	20.26	0.72	20.16	0.78	20.04	0.84	19.92
24	25.80	0.63	24.54	0.68	24.44	0.73	24.34	0.79	24.22	0.79	24.22	0.85	24.10	0.92	23.96

Cast Iron Pipe - AWWA Standard

		Class A 100 Ft. 43 PSIG			Class B 200 Ft. 86 PSIG			Class C 300 Ft. 130 PSIG			Class D 400 Ft. 173 PSIG		
Pipe Size	O.D.	WALL	I.D.	O.D.	WALL	I.D.	O.D.	WALL	I.D.	O.D.	WALL	I.D.	
3	3.80	0.39	3.02	3.96	0.42	3.12	3.96	0.45	3.06	3.96	0.48	3.00	
4	4.80	0.42	3.96	5.00	0.45	4.10	5.00	0.48	4.04	5.00	0.52	3.96	
6	6.90	0.44	6.02	7.10	0.48	6.14	7.10	0.51	6.08	7.10	0.55	6.00	
8	9.05	0.46	8.13	9.05	0.51	8.03	9.30	0.56	8.18	9.30	0.60	8.10	
10	11.10	0.50	10.10	11.10	0.57	9.96	11.40	0.62	10.16	11.40	0.68	10.04	
12	13.20	0.54	12.12	13.20	0.62	11.96	13.50	0.68	12.14	13.50	0.75	12.00	
14	15.30	0.57	14.16	15.30	0.66	13.98	15.65	0.74	14.17	15.65	0.82	14.01	
16	17.40	0.60	16.20	17.40	0.70	16.00	17.80	0.80	16.20	17.80	0.89	16.02	
18	19.50	0.64	18.22	19.50	0.75	18.00	19.92	0.87	18.18	19.92	0.96	18.00	
20	21.60	0.67	20.26	21.60	0.80	20.00	22.06	0.92	20.22	22.06	1.03	20.00	
24	25.80	0.76	24.28	25.80	0.89	24.02	26.32	1.04	24.22	26.32	1.16	24.00	
30	31.74	0.88	29.98	32.00	1.03	29.94	32.40	1.20	30.00	32.74	1.37	30.00	
36	37.96	0.99	35.98	38.30	1.15	36.00	38.70	1.36	39.98	39.16	1.58	36.00	
42	44.20	1.10	42.00	44.50	1.28	41.94	45.10	1.54	42.02	45.58	1.78	42.02	
48	50.50	1.26	47.98	50.80	1.42	47.96	51.40	1.71	47.98	51.98	1.96	48.06	
54	56.66	1.35	53.96	57.10	1.55	54.00	57.80	1.90	54.00	58.40	2.23	53.94	
60	62.80	1.39	60.02	63.40	1.67	60.06	64.20	2.00	60.20	64.82	2.38	60.06	
72	75.34	1.62	72.10	76.00	1.95	72.10	76.88	2.39	72.10				
84	87.54	1.72	84.10	88.54	2.22	84.10							

	Class E 500 Ft. 217 PSIG			600	Class F 600 Ft. 260 PSIG			Class G 700 Ft. 304 PSIG			Class H 800 Ft. 347 PSIG		
Pipe											r		
Size	O.D.	WALL	I.D.	O.D.	WALL	I.D.	O.D.	WALL	I.D.	O.D.	WALL	I.D.	
6	7.22	0.58	6.06	7.22	0.61	6.00	7.38	0.65	6.08	7.38	0.69	6.00	
8	9.42	0.66	8.10	9.42	0.71	8.00	9.60	0.75	8.10	9.60	0.80	8.00	
10	11.60	0.74	10.12	11.60	0.80	10.00	11.84	0.86	10.12	11.84	0.92	10.00	
12	13.78	0.82	12.14	13.78	0.89	12.00	14.08	0.97	12.14	14.08	1.04	12.00	
14	15.98	0.90	14.18	15.98	0.99	14.00	16.32	1.07	14.18	16.32	1.16	14.00	
16	18.16	0.98	16.20	18.16	1.08	16.00	18.54	1.18	16.18	18.54	1.27	16.00	
18	20.34	1.07	18.20	20.34	1.17	18.00	20.78	1.28	18.22	20.78	1.39	18.00	
20	22.54	1.15	20.24	22.54	1.27	20.00	23.02	1.39	20.24	23.02	1.51	20.00	
24	26.90	1.31	24.28	26.90	1.45	24.00	27.76	1.75	24.26	27.76	1.88	24.00	
30	33.10	1.55	30.00	33.46	1.73	30.00							
36	39.60	1.80	36.00	40.04	2.02	36.00							



Copper Tubing

Pipe	Size				L		м			Coppe	er & Bras	s Pipe	Aluminum		
Size	O.D.	I.D.	WALL	O.D.	I.D.	WALL	O.D.	I.D.	WALL	0.D.	I.D.	WALL	O.D.	I.D.	WALL
1⁄2"	0.625	0.527	0.049	0.625	0.545	0.040	0.625	0.569	0.028						
3⁄4"	0.875	0.745	0.065	0.875	0.785	0.045	0.875	0.811	0.032						
1"	1.125	0.995	0.065	1.125	1.025	0.050	1.125	1.055	0.035						
1 ¼"	1.375	1.245	0.065	1.375	1.265	0.055	1.375	1.291	0.042						
1 ½"	1.625	1.481	0.072	1.625	1.505	0.060	1.625	1.527	0.049						
2"	2.125	1.959	0.083	2.125	1.985	0.070	2.125	2.009	0.058	2.375	2.062	0.157			
2 1/2	2.625	2.435	0.095	2.625	2.465	0.080	2.625	2.495	0.065	2.875	2.500	0.188	2.500	2.400	0.050
3"	3.125	2.907	0.109	3.125	2.945	0.090	3.125	2.981	0.072	3.500	3.062	0.219	3.000	2.900	0.050
3 ½"	3.625	3.385	0.120	3.625	3.425	0.100	3.625	3.459	0.083	4.000	3.500	0.250			
4"	4.125	3.857	0.134	4.125	3.905	0.110	4.125	3.935	0.095	4.500	3.935	0.095	4.000	4.000	0.250
4 ½"													5.000	4.500	0.250
5"	5.125	4.805	0.160	5.125	4.875	0.125	5.125	4.907	0.109	5.563	5.063	0.250	5.000	4.874	0.063
6"	6.125	5.741	0.192	6.125	5.845	0.140	6.125	5.881	0.122	6.625	6.125	0.250	6.000	5.874	0.063
7"										7.625	7.062	0.282	7.000	6.844	0.078
8"	8.125	7.583	0.271	8.125	7.725	0.200	8.125	7.785	0.170	8.625	8.000	0.313	8.000	7.812	0.094
10"	10.125	9.449	0.338	10.125	9.625	0.250	10.125	9.701	0.212	10.000	9.812	0.094			
12"	12.125	11.315	0.405	12.125	11.565	0.280	12.125	11.617	0.254						

HDPE

Pipe	0.0	C)R 7	D	R 7.3		R 9	D	R 11	DR	13.5	DR	15.5
Size	OD	Wall	ID	Wall	1 D	Wall	ID	Wall	ID	Wall	ID	Wall	ID
2"	2.375"	0.339"	1.656"	0.325"	1.685"	0.264"	1.816°	0.216 ^π	1.917"	0.176"	2.002"	0.153"	2.050"
3"	3.500"	0.500"	2.440°	0.479"	2.484"	0.389"	2.676°	0.318 ⁿ	2.825"	0.259"	2.950"	0.226°	3.021"
4"	4.500"	0.643"	3.137"	0.616"	3.193"	0.500"	3.440"	0.409"	3.633"	0.333"	3.793"	0.290"	3.885"
5"	5.563"	0.795"	3.878"	0.762"	3.947"	0.618"	4.253°	0.506 [∞]	4.491"	0.412"	4.689"	0.347°	4.640"
6"	6.625"	0.946"	4.619°	0.908"	4.701"	0.736"	5.064"	0.602 ^π	5.348"	0.491"	5.585°	0.359°	4.802"
7"	7.125"	1.018"	4.967°	0.976"	5.056"	0.792"	5.447°	0.648 ^π	5.752"	0.528"	6.005"	0.427"	5.719"
8"	8.625"	1.232"	6.013°	1.182"	6.120"	0.958"	6.593"	0.784"	6.963"	0.639"	7.271 ^ª	0.460"	6.150"
10"	10.750"	1.536"	7.494"	1.473"	7.628"	1.194"	8.218"	0.977"	8.678"	0.7 96 "	9.062"	0.556"	7.445"
12"	12.750"	1.821"	8.889°	1.747"	9.047"	1.417"	9.747°	1.159 ^π	10.293°	0.944"	10.748"	0.694"	9.280"
14"	14.000"	2.000"	9.760"	1.918"	9.934"	1.556"	10.702"	1.273 ^π	11.302°	1.037"	11.801"	0.823"	11.006"
16"	15.00"	2,286"	11.154"	2,192"	11.353"	1.778"	12,231"	1.455 [¤]	12.91 5 "	1,185"	13.487"	0.903 ⁿ	12.085 ⁿ
18"	18.00"	2.571"	12.549"	2.466"	12.773"	2.000"	13.760"	1.636 ^π	14.531°	1.333"	15.173"	1.032 ⁿ	13.812 ¹¹
20"	20.00"	2.857"	13. 9 43"	2.740"	14.192"	2.222"	15.289"	1.818 ^π	16.145°	1.481"	16.85 9 "	1.161"	15.538"
22"	22.00"	3.143"	15.337"	3.014"	15.611"	2.444"	16.818"	2.000"	17.760"	1.630"	18.545"	1.290"	17.265"
24"	24.00"	3.429"	16.731"	3.288"	17.030"	2.667"	18.347"	2.182 ^u	19.375°	1.778"	20.231"	1.419 ⁿ	18.99 1 ⁿ
26"	26.00"			3.562"	18.449"	2.889"	19.876"	2.364 [≖]	20.989°	1.926"	21.917"	1.548"	20.717 ¹⁷
28"	28.00"]				3.111"	21.404"	2.545 [≖]	22.604"	Z.074"	23.603"	1.677"	22.444 ["]
30"	30.00"]		_	_	3.333"	22. 9 33"	2.727 [≖]	24.218"	2.222"	25.289"	1.806°	24.170"
32"	32.00"]				3.556″	24.462"	2.909"	25.833"	2.370"	26.975"	1.935"	25.897"
34"	34.00"]						3.091"	27.447"	2.519"	28.661"	2.065"	27.623"
36"	36.00"]			_		—	3.273 [™]	29.062°	2.667"	30.347"	2.1 9 4"	29.350"
42"	42.00"]		-	_	_	_			3.111"	35.404"	2.323"	31.076"
48"	48.00"			_	_	_		·		3.556"	40.462"	2.710"	36.255"



Pipe Size	OD	DR	14	DR18		DR	-21	DR25		
		Wall	ID	Wall	ID	Wall	ID	Wall	ID	
4	4.80	0.343	4.114	0.267	4.266			0.192	4.416	
6	6.90	0.493	5.914	0.383	6.134			0.276	6.348	
8	9.05	0.646	7.758	0.503	8.044			0.362	8.326	
10	11.10	0.793	9.514	0.617	9.866			0.444	10.212	
12	13.20	0.943	11.314	0.733	11.734			0.528	12.144	
14	15.30			0.850	13.600	0.729	13.842	0.612	14.076	
16	17.40			0.967	15.466	0.829	15.742	0.696	16.008	
18	19.50			1.083	17.334	0.929	17.642	0.780	17.94	
20	21.60			1.200	19.200	1.029	19.542	0.864	19.872	
24	25.80			1.433	22.934	1.229	23.342	1.032	23.736	

C900/C905 PVC AWWA Water Distribution Pipe (Blue)



Substance	Form Index	Specific Gravity	Sound Speed	v/°C - m/s/°CΔ
			m/sec.	
Acetic anhydride (22)	(CH3CO)2O	1.082 (20°C)	1180	2.5
Acetic acid, anhydride (22)	(CH3CO)2O	1.082 (20°C)	1180	2.5
Acetic acid, nitrile	C2H3N	0.783	1290	4.1
Acetic acid, ethyl ester (33)	C4H8O2	0.901	1085	4.4
Acetic acid, methyl ester	C3H6O2	0.934	1211	
Acetone	C3H6O	0.791	1174	4.5
Acetonitrile	C2H3N	0.783	1290	4.1
Acetonylacetone	C6H10O2	0.729	1399	3.6
Acetylene dichloride	C2H2C12	1.26	1015	3.8
Acetylene tetrabromide (47)	C2H2Br4	2.966	1027	
Acetylene tetrachloride (47)	C2H2Cl4	1.595	1147	
Alcohol	C2H6O	0.789	1207	4.0
Alkazene-13	C15H24	0.86	1317	3.9
Alkazene-25	C10H12Cl2	1.20	1307	3.4
2-Amino-ethanol	C2H7NO	1.018	1724	3.4
2-Aminotolidine (46)	C7H9N	0.999 (20°C)	1618	
4-Aminotolidine (46)	C7H9N	0.966 (45°C)	1480	
Ammonia (35)	NH3	0.771	1729	6.68
Amorphous Polyolefin		0.98	962.6	
t-Amyl alcohol	C5H12O	0.81	1204	
Aminobenzene (41)	C6H5NO2	1.022	1639	4.0
Aniline (41)	C6H5NO2	1.022	1639	4.0
Argon (45)	Ar	1.400 (-188°C)	853	
Azine	C6H5N	0.982	1415	4.1
Benzene (29,40,41)	C6H6	0.879	1306	4.65
Benzol(29,40,41)	C6H6	0.879	1306	4.65
Bromine (21)	Br2	2.928	889	3.0
Bromo-benzene (46)	C6H5Br	1.522	1170	
1-Bromo-butane (46)	C4H9Br	1.276 (20°C)	1019	
Bromo-ethane (46)	C ₂ H ₅ Br	1.460 (20°C)	900	
Bromoform (46,47)	СНВгз	2.89 (20°C)	918	3.1
n-Butane (2)	C4H10	0.601 (0°C)	1085	5.8
2-Butanol	C4H10O	0.81	1240	3.3
sec-Butylalcohol	C4H10O	0.81	1240	3.3
n-Butyl bromide (46)	C4H9Br	1.276 (20°C)	1019	
n-Butyl chloride (22,46)	C4H9CI	0.887	1140	4.57
tert Butyl chloride	C4H9CI	0.84	984	4.2
Butyl oleate	C22H42O2		1404	3.0
2,3 Butylene glycol	C4H10O2	1.019	1484	1.51
Cadmium (7)	Cd		2237.7	-
Carbinol (40,41)	CH4O	0.791 (20°C)	1076	2.92
Carbitol	C6H14O3	0.988	1458	
Carbon dioxide (26)	CO ₂	1.101 (-37°C)	839	7.71
Carbon disulphide	CS2	1.261 (22°C)	1149	

APPENDIX C – Liquid Speed of Sound



Substance	Form Index	Specific Gravity	Sound Speed m/sec.	v/°C - m/s/°CΔ
Carbon tetrachloride(33,35,47)	CCl4	1.595 (20°C)	926	2.48
Carbon tetrafluoride (14)	CF4	1.75 (-150⁰C)	875.2	6.61
Cetane (23)	C16H34	0.773 (20°C)	1338	3.71
Chloro-benezene	C6H5Cl	1.106	1273	3.6
1-Chloro-butane (22,46)	C4H9Cl	0.887	1140	4.57
Chloro-diFluoromethane (3) (Freon 22)	CHCIF2	1.491 (-69ºC)	893.9	4.79
Chloroform (47)	CHCl3	1.489	979	3.4
1-Chloro-propane (47)	C3H7CI	0.892	1058	
Chlorotrifluoromethane (5)	CCIF3		724	5.26
Cinnamaldehyde	C9H8O	1.112	1554	3.2
Cinnamic aldehyde	C9H8O	1.112	1554	3.2
Colamine	C2H7NO	1.018	1724	3.4
o-Cresol (46)	C7H8O	1.047 (20°C)	1541	
m-Cresol (46)	C7H8O	1.034 (20°C)	1500	
Cyanomethane	C2H3N	0.783	1290	4.1
Cyclohexane (15)	C6H12	0.779 (20°C)	1248	5.41
Cyclohexanol	C6H12O	0.962	1454	3.6
Cyclohexanone	C6H10O	0.948	1423	4.0
Decane (46)	C10H22	0.730	1252	
1-Decene (27)	C10H20	0.746	1235	4.0
n-Decylene (27)	C10 H20	0.746	1235	4.0
Diacetyl	C4H6O2	0.99	1236	4.6
Diamylamine	C10H23N		1256	3.9
1,2 Dibromo-ethane (47)	C2H4Br2	2.18	995	
trans-1,2-Dibromoethene(47)	C2H2Br2	2.231	935	
Dibutyl phthalate	C8H22O4		1408	
Dichloro-t-butyl alcohol	C4H8Cl2O		1304	3.8
2,3 Dichlorodioxane	C2H6Cl2O2		1391	3.7
Dichlorodifluoromethane (3) (Freon 12)	CCl ₂ F ₂	1.516 (-40°C)	774.1	4.24
1,2 Dichloro ethane (47)	C2H4Cl2	1.253	1193	
cis 1,2-Dichloro-Ethene(3,47)	C2H2Cl2	1.284	1061	
trans 1,2-Dichloro-ethene(3,47)	C2H2Cl2	1.257	1010	
Dichloro-fluoromethane (3) (Freon 21)	CHCl ₂ F	1.426 (0°C)	891	3.97
1-2-Dichlorohexafluoro cyclobutane (47)	C4Cl2F6	1.654	669	
1-3-Dichloro-isobutane	C4H8Cl2	1.14	1220	3.4
Dichloro methane (3)	CH2Cl2	1.327	1070	3.94
1,1-Dichloro-1,2,2,2 tetra fluoroethane	CCIF2-CCIF2	1.455	665.3	3.73
Diethyl ether	C4H10O	0.713	985	4.87
Diethylene glycol, monoethyl ether	C6H14O3	0.988	1458	
Diethylenimide oxide	C4H9NO	1.00	1442	3.8
1,2-bis(DiFluoramino) butane (43)	C4H8(NF2)2	1.216	1000	
1,2bis(DiFluoramino)- 2-methylpropane (43)	C4H9(NF2)2	1.213	900	
1,2bis(DiFluoramino) propane (43)	C3H6(NF2)2	1.265	960	
2,2bis(DiFluoramino) propane (43)	C3H6(NF2)2	1.254	890	



Substance	Form Index	Specific Gravity	Sound Speed m/sec.	v/°C - m/s/°C∆
2,2-Dihydroxydiethyl ether	C4H10O3	1.116	1586	2.4
Dihydroxyethane	C2H6O2	1.113	1658	2.1
1,3-Dimethyl-benzene (46)	C8H10	0.868 (15°C)	1343	
1,2-1.0Dimethyl-benzene(29,46)	C8H10	0.897 (20°C)	1331.5	4.1
1,4-Dimethyl-benzene (46)	C8H10		1334	
2,2-Dimethyl-butane (29,33)	C6H14	0.649 (20°C)	1079	
Dimethyl ketone	СзН6О	0.791	1174	4.5
Dimethyl pentane (47)	C7H16	0.674	1063	
Dimethyl phthalate	C8H10O4	1.2	1463	
Diiodo-methane	CH2l2	3.235	980	
Dioxane	C4H8O2	1.033	1376	
Dodecane (23)	C12H26	0.749	1279	3.85
1,2-Ethanediol	C2H6O2	1.113	1658	2.1
Ethanenitrile	C2H3N	0.783	1290	
Ethanoic anhydride (22)	(CH3CO)2O	1.082	1180	
Ethanol	C2H6O	0.789	1207	4.0
Ethanol amide	C2H7NO	1.018	1724	3.4
Ethoxyethane	C4H10O	0.713	985	4.87
Ethyl acetate (33)	C4H8O2	0.901	1085	4.4
Ethyl alcohol	C2H6O	0.789	1207	4.0
Ethyl benzene (46)	C8H10	0.867(20°C)	1338	
Ethyl bromide (46)	C2H5Br	1.461 (20°C)	900	
Ethyliodide (46)	C2H5I	1.950 (20°C)	876	
Ether	C4H10O	0.713	985	4.87
Ethyl ether	C4H10O	0.713	985	4.87
Ethylene bromide (47)	C2H4Br2	2.18	995	
Ethylene chloride (47)	C2H4Cl2	1.253	1193	
Ethylene glycol	C2H6O2	1.113	1658	2.1
50% Glycol/ 50% H2O			1578	
d-Fenochone	C10H16O	0.947	1320	
d-2-Fenechanone	C10H16O	0.947	1320	
Fluorine	F	0.545 (-143ºC)	403	11.31
Fluoro-benzene (46)	C6H5F	1.024 (20°C)	1189	
Formaldehyde, methyl ester	C2H4O2	0.974	1127	4.02
Formamide	CH3NO	1.134 (20°C)	1622	2.2
Formic acid, amide	CH3NO	1.134 (20°C)	1622	
Freon R12			774	
Furfural	C5H4O2	1.157	1444	
Furfuryl alcohol	C5H6O2	1.135	1450	3.4
Fural	C5H4O2	1.157	1444	3.7
2-Furaldehyde	C5H4O2	1.157	1444	3.7
2-Furancarboxaldehyde	C5H4O2	1.157	1444	3.7
2-Furyl-Methanol	C5H6O2	1.135	1450	3.4
Gallium	Ga	6.095	2870 (@30°C)	



Substance	Form Index	Specific Gravity	Sound Speed m/sec.	v/°C - m/s/°C∆
Glycerin	СзН8Оз	1.26	1904	2.2
Glycerol	СзН8Оз	1.26	1904	2.2
Glycol	C2H6O2	1.113	1658	2.1
Helium (45)	He4	0.125(-268.8°C)	183	
Heptane (22,23)	C7H16	0.684 (20°C)	1131	4.25
n-Heptane (29,33)	C7H16	0.684 (20°C)	1180	4.0
Hexachloro-Cyclopentadiene(47)	C5Cl6	1.7180	1150	
Hexadecane (23)	C16H34	0.773 (20°C)	1338	3.71
Hexalin	C6H12O	0.962	1454	3.6
Hexane (16,22,23)	C6H14	0.659	1112	2.71
n-Hexane (29,33)	C6H14	0.649 (20°C)	1079	4.53
2,5-Hexanedione	C6H10O2	0.729	1399	3.6
n-Hexanol	C6H14O	0.819	1300	3.8
Hexahydrobenzene (15)	C6H12	0.779	1248	5.41
Hexahydrophenol	C6H12O	0.962	1454	3.6
Hexamethylene (15)	C6H12	0.779	1248	5.41
Hydrogen (45)	H2	0.071 (-256°C)	1187	
2-Hydroxy-toluene (46)	C7H8O	1.047 (20°C)	1541	
3-Hydroxy-tolune (46)	C7H8O	1.034 (20°C)	1500	
lodo-benzene (46)	C6H5I	1.823	1114	
lodo-ethane (46)	C2H5I	1.950 (20°C)	876	
lodo-methane	CH3I	2.28 (20°C)	978	
Isobutyl acetate (22)	C6H12O		1180	4.85
Isobutanol	C4H10O	0.81 (20°C)	1212	
Iso-Butane			1219.8	
Isopentane (36)	C5H12	0.62 (20°C)	980	4.8
Isopropanol (46)	C3H8O	0.785 (20°C)	1170	
Isopropyl alcohol (46)	C3H8O	0.785 (20°C)	1170	
Kerosene		0.81	1324	3.6
Ketohexamethylene	C6H10O	0.948	1423	4.0
Lithium fluoride (42)	LiF		2485	1.29
Mercury (45)	Hg	13.594	1449	
Mesityloxide	C6H16O	0.85	1310	
Methane (25,28,38,39)	CH4	0.162	405(-89.15°C)	17.5
Methanol (40,41)	CH4O	0.791 (20°C)	1076	2.92
Methyl acetate	C3H6O2	0.934	1211	
o-Methylaniline (46)	C7H9N	0.999 (20°C)	1618	
4-Methylaniline (46)	C7H9N	0.966 (45°C)	1480	
Methyl alcohol (40,44)	CH4O	0.791 (20°C)	1076	2.92
Methyl benzene (16,52)	C7H8	0.867	1328	4.27
2-Methyl-butane (36)	C5H12	0.62 (20°C)	980	
Methyl carbinol	C2H6O	0.789	1207	4.0
Methyl-chloroform (47)	C2H3Cl3	1.33	985	
Methyl-cyanide	C2H3N	0.783	1290	



Substance	Form Index	Specific Gravity	Sound Speed m/sec.	v/°C - m/s/°C∆	
3-Methyl cyclohexanol	C7H14O	0.92	1400		
Methylene chloride (3)	CH2Cl2	1.327	1070	3.94	
Methylene iodide	CH2l2	3.235	980		
Methyl formate (22)	C2H4O2	0.974 (20°C)	1127	4.02	
Methyl iodide	CH3I	2.28 (20°C)	978		
2-Methylphenol (46)	C7H8O	1.047 (20°C)	1541		
3-Methylphenol (46)	C7H8O	1.034 (20°C)	1500		
Milk, homogenized			1548		
Morpholine	C4H9NO	1.00	1442	3.8	
Naphtha		0.76	1225		
Natural Gas (37)		0.316 (-103ºC)	753		
Neon (45)	Ne	1.207 (-246°C)	595		
Nitrobenzene (46)	C6H5NO2	1.204 (20°C)	1415		
Nitrogen (45)	N2	0.808 (-199°C)	962		
Nitromethane (43)	CH3NO2	1.135	1300	4.0	
Nonane (23)	C9H2O	0.718 (20°C)	1207	4.04	
1-Nonene (27)	C9H18	0.736 (20°C)	1207	4.0	
Octane (23)	C8H18	0.703	1172	4.14	
n-Octane (29)	C8H18	0.704 (20°C)	1212.5	3.50	
1-Octene (27)	C8H16	0.723 (20°C)	1175.5	4.10	
Oil of Camphor Sassafrassy			1390	3.8	
Oil, Car (SAE 20a.30)	1.74		870		
Oil, Castor	C11H10O10	0.969	1477	3.6	
Oil, Diesel		0.80	1250		
Oil, Fuel AA gravity		0.99	1485	3.7	
Oil (Lubricating X200)			1530	5019.9	
Oil (Olive)		0.912	1431	2.75	
Oil (Peanut)		0.936	1458		
Oil (Sperm)		0.88	1440		
Oil, 6			1509		
2,2-Oxydiethanol	C4H10O3	1.116	1586	2.4	
Oxygen (45)	O2	1.155 (-186ºC)	952		
Pentachloro-ethane (47)	C2HCl5	1.687	1082		
Pentalin (47)	C2HCl5	1.687	1082		
Pentane (36)	C5H12	0.626 (20°C)	1020		
n-Pentane (47)	C5H12	0.557	1006		
Perchlorocyclopentadiene(47)	C5Cl6	1.718	1150		
Perchloro-ethylene (47)	C2Cl4	1.632	1036		
Perfluoro-1-Hepten (47)	C7F14	1.67	583		
Perfluoro-n-Hexane (47)	C6F14	1.672	508		
Phene (29,40,41)	C6H6	0.879	1306	4.65	
ß-Phenyl acrolein	C9H8O	1.112	1554	3.2	
Phenylamine (41)	C6H5NO2	1.022	1639	4.0	



Substance	Form Index	Specific Gravity	Sound Speed m/sec.	v/°C - m/s/°C∆	
Phenyl bromide (46)	C6H₅Br	1.522	1170		
Phenyl chloride	C6H5CI	1.106	1273	3.6	
Phenyl iodide (46)	C6H5I	1.823	1114		
Phenyl methane (16,52)	C7H8	0.867 (20°C)	1328	4.27	
3-Phenyl propenal	C9H8O	1.112	1554	3.2	
Phthalardione	C8H4O3		1125		
Phthalic acid, anhydride	C8H4O3		1125		
Phthalic anhydride	C8H4O3		1125		
Pimelic ketone	C6H10O	0.948	1423	4.0	
Plexiglas, Lucite, Acrylic			2651		
Polyterpene Resin		0.77	1099.8		
Potassium bromide (42)	Kbr		1169	0.71	
Potassium fluoride (42)	KF		1792	1.03	
Potassium iodide (42)	KI		985	0.64	
Potassium nitrate (48)	KNO3	1.859 (352°C)	1740.1	1.1	
Propane (2,13)(-45 to -130°C)	СзНв	0.585 (-45°C)	1003	5.7	
1,2,3-Propanetriol	СзН8Оз	1.26	1904	2.2	
1-Propanol (46)	C3H8O	0.78 (20°C)	1222		
2-Propanol (46)	СзН8О	0.785 (20°C)	1170		
2-Propanone	СзН6О	0.791	1174	4.5	
Propene (17,18,35)	C3H6	0.563 (-13ºC)	963	6.32	
n-Propyl acetate (22)	C5H10O2	1280 (2°C)	4.63		
n-Propyl alcohol	СзН8О	0.78 (20°C)	1222		
Propylchloride (47)	C3H7CI	0.892	1058		
Propylene (17,18,35)	СзН6	0.563 (-13°C)	963	6.32	
Pyridine	C6H5N	0.982	1415	4.1	
Refrigerant 11 (3,4)	CCl3F	1.49	828.3	3.56	
Refrigerant 12 (3)	CCl ₂ F ₂	1.516 (-40ºC)	774.1	4.24	
Refrigerant 14 (14)	CF4	1.75 (-150ºC)	875.24	6.61	
Refrigerant 21 (3)	CHCl2F	1.426 (0°C)	891	3.97	
Refrigerant 22 (3)	CHCIF2	1.491 (-69°C)	893.9	4.79	
Refrigerant 113 (3)	CCI2F-CCIF2	1.563	783.7	3.44	
Refrigerant 114 (3) Refrigerant 115 (3)	CCIF2-CCIF2 C2CIF5	1.455	665.3 656.4	3.73	
		(22 (2222)		4.42	
Refrigerant C318 (3)	C4F8	1.62 (-20°C)	574	3.88	
Selenium (8)	Se	0.000	1072	0.68	
Silicone (30 cp)		0.993	990		
Sodium fluoride (42)	NaF	0.877	2082	1.32	
Sodium nitrate (48)	NaNO3	1.884 (336°C)	1763.3	0.74	
Sodium nitrite (48)	NaNO ₂	1.805 (292°C)	1876.8		
Solvesso 3		0.877	1370	3.7	
Spirit of wine	C2H6O	0.789	1207	4.0	
Sulphur (7,8,10)	S		1177	-1.13	
Sulphuric acid (1)	H2SO4	1.841	1257.6	1.43	



Substance	Form Index	Specific Gravity	Sound Speed m/sec.	v/°C - m/s/°CΔ	
Tellurium (7)	Te		991	0.73	
1,1,2,2-Tetrabromo-ethane(47)	C ₂ H ₂ Br ₄	2.966120	1027		
1,1,2,2-Tetrachloro-ethane(67)	C2H2Cl4	1.595	1147		
Tetrachloroethane (46)	C2H2Cl4	1.553 (20°C)	1170		
Tetrachloro-ethene (47)	C2Cl4	1.632	1036		
Tetrachloro-methane (33,47)	CCl4	1.595 (20°C)	926		
Tetradecane (46)	C14H3O	0.763 (20°C)	1331		
Tetraethylene glycol	C8H18O5	1.123	1586/5203.4	3.0	
Tetrafluoro-methane (14) (Freon 14)	CF4	1.75 (-150⁰C)	875.24	6.61	
Tetrahydro-1,4-isoxazine	C4H9NO		1442	3.8	
Toluene (16,52)	C7H8	0.867 (20°C)	1328	4.27	
o-Toluidine (46)	C7H9N	0.999 (20°C)	1618		
p-Toluidine (46)	C7H9N	0.966 (45°C)	1480		
Toluol	C7H8	0.866	1308	4.2	
Tribromo-methane (46,47)	CHBr ₃	2.89 (20°C)	918		
1,1,1-Trichloro-ethane (47)	C2H3Cl3	1.33	985		
Trichloro-ethene (47)	C2HCl3	1.464	1028		
Trichloro-fluoromethane (3) (Freon 11)	CCI3F	1.49	828.3	3.56	
Trichloro-methane (47)	CHCl3	1.489	979	3.4	
1,1,2-Trichloro-1,2,2-Trifluoro-Ethane	CCl ₂ F-CClF ₂	1.563	783.7		
Triethyl-amine (33)	C6H15N	0.726	1123	4.47	
Triethylene glycol	C6H14O4	1.123	1608	3.8	
1,1,1-Trifluoro-2-Chloro-2-Bromo-Ethane	C ₂ HCIBrF ₃	1.869	693		
1,2,2-Trifluorotrichloro- ethane (Freon 113)	CCl ₂ F-CClF ₂	1.563	783.7	3.44	
d-1,3,3-Trimethylnor- camphor	C10H16O	0.947	1320		
Trinitrotoluene (43)	C7H5(NO2)3	1.64	1610		
Turpentine		0.88	1255		
Unisis 800		0.87	1346		
Water, distilled (49,50)	H2O	0.996	1498	-2.4	
Water, heavy	D ² O		1400		
Water, sea		1.025	1531	-2.4	
Wood Alcohol (40,41)	CH4O	0.791 (20°C)	1076	2.92	
Xenon (45)	Xe		630		
m-Xylene (46)	C8H10	0.868 (15°C)	1343		
o-Xylene (29,46)	C8H10	0.897 (20°C)	1331.5	4.1	
p-Xylene (46)	C8H10		1334		
Xylene hexafluoride	C8H4F6	1.37	879		
Zinc (7)	Zn		3298		



Appendi<u>x</u> D

	Sonic Velocity Relative to Temperature of Pure Water								
Temp °F	Temp °C	Velocity ft/s	Temp °F	Temp °C	Velocity ft/s	Temp °F	Temp °C	Velocity ft/s	
0.0	-17.8	4240	100.0	37.8	5003	200.0	93.3	5080	
2.0	-16.7	4267	102.0	38.9	5010	202.0	94.4	5077	
4.0	-15.6	4293	104.0	40.0	5016	204.0	95.6	5075	
6.0	-14.4	4319	106.0	41.1	5022	206.0	96.7	5077	
8.0	-13.3	4344	108.0	42.2	5028	208.0	97.8	5069	
10.0	-12.2	4368	110.0	43.3	5033	210.0	98.9	5066	
12.0	11.0	4392	112.0	44.4	5038	212.0	100.0	5063	
14.0	10.0	4416	114.0	45.6	5043	214.0	101.1	5059	
16.0	-8.9	4438	116.0	46.7	5048	216.0	102.2	5056	
18.0	-7.8	4460	118.0	47.8	5052	218.0	103.3	5052	
20.0	-6.7	4482	120.0	48.9	5057	220.0	104.4	5049	
22.0	-5.6	4503	122.0	50.0	5061	222.0	105.6	5045	
24.0	-4.4	4524	124.0	51.1	5065	224.0	106.7	5041	
26.8	-3.3	4544	126.0	52.2	5068	226.0	107.8	5037	
28.0	-2.2	4563	128.0	53.3	5072	228.0	108.9	5033	
30.0	-1.1	4582	130.0	54.4	5075	230.0	110.0	5029	
32.0	0.0	4601	132.0	55.6	5078	232.0	111.1	5024	
34.0	1.1	4619	134.0	56.7	5081	234.0	112.2	5020	
36.0	2.2	4637	136.0	57.8	5084	236.0	113.3	5015	
38.0	3.3	4654	138.0	58.9	5086	238.0	114.4	5011	
40.0	4.4	4671	140.0	60.0	5089	240.0	115.6	5006	
42.0	5.6	4687	142.0	61.1	5091	242.0	116.7	5001	
44.0	6.7	4703	144.0	62.2	5093	244.0	117.8	4996	
46.0	7.8	4719	146.0	63.3	5094	246.0	118.9	4991	
48.0	8.9	4734	148.0	64.4	5096	248.0	120.0	4986	
50.0	10.0	4748	150.0	65.6	5097	250.0	121.1	4981	
52.0	11.1	4763	152.0	66.7	5098	260.0	126.7	4944	
54.0	12.2	4776	154.0	67.8	5099	270.0	132.2	4911	
56.0	13.3	4790	156.0	68.9	5100	280.0	137.8	4879	
58.0	14.4	4803	158.0	70.0	5101	290.0	143.3	4843	
60.0	.15.56	4816	160.0	71.1	5102	300.0	148.9	4806	
62.0	16.7	4828	162.0	72.2	5102	310.0	154.4	4767	
64.0	17.9	4840	164.0	73.3	5102	320.0	160.0	4724	
66.0	18.9	4852	166.0	74.4	5102	330.0	165.6	4678	
68.0	20.0	4863	168.0	75.6	5102	340.0	171.1	4633	
70.0	21.1	4874	170.0	76.7	5102	350.0	176.7	4587	
72.0	22.2	4885	172.0	77.8	5101	360.0	182.2	4537	
74.0	23.3	4895	174.0	78.9	5101	370.0	187.8	4488	
76.0	24.4	4905	176.0	80.0	5100	380.0	193.3	4439	
78.0	25.6	4915	178.0	81.1	5099	390.0	198.9	4386	
80.0	26.7	4925	180.0	82.2	5098	400.0	204.4	4331	
82.0	27.8	4934	182.0	83.3	5097	410.0	210.0	4272	
84.0	28.9	4943	184.0	84.4	5096	420.0	215.6	4209	
86.0	30.0	4951	186.0	85.6	5094	430.0	221.1	4147	
88.0	31.1	4959	188.0	86.7	5093	440.0	226.7	4081	
90.0	32.2	4967	190.0	87.8	5091	450.0	232.2	4003	
92.0	33.3	4975	192.0	88.9	5089	460.0	237.8	3937	
94.0	34.4	4983	194.0	90.0	5087	470.0	243.3	3871	
96.0	35.6	4990	196.0	91.1	5085	480.0	248.9	3806	
98.0	36.7	4997	198.0	92.2	5082	490.0	254.4	3740	



Sonic Velocity Relative to Temperature of Pure Water Temp °F Temp °C Velocity m/s Temp °F Temp °C Velocity m/s Temp °F Temp °C Velocity m/s								
Temp °F	Temp °C	Velocity m/s	Temp °F	Temp °C	Velocity m/s	Temp °F	Temp °C	Velocity m/
0.0	-17.8	1292.45	100.0	37.8	1525.03	200.0	93.3	1548.38
2.0	-16.7	1300.64	102.0	38.9	1526.99	202.0	94.4	1547.60
4.0	-15.6	1308.63	104.0	40.0	1528.86	204.0	95.6	1546.78
6.0	-14.4	1316.44	106.0	41.1	1530.67	206.0	96.7	1547.60
8.0	-13.3	1324.06	108.0	42.2	1532.4	208.0	97.8	1545.02
10.0	-12.2	1331.50	110.0	43.3	1534.06	210.0	98.9	1544.08
12.0	11.0	1338.77	112.0	44.4	1535.64	212.0	100.0	1543.11
14.0	10.0	1345.86	114.0	45.6	1537.16	214.0	101.1	1542.10
16.0	-8.9	1352.78	116.0	46.7	1538.61	216.0	102.2	1541.05
18.0	-7.8	1359.53	118.0	47.8	1539.99	218.0	103.3	1539.97
20.0	-6.7	1366.12	120.0	48.9	1541.30	220.0	104.4	1538.85
22.0	-5.6	1372.55	122.0	50.0	1542.55	222.0	105.6	1537.70
24.0	-4.4	1378.82	124.0	51.1	1543.74	224.0	106.7	1536.51
26.8	-3.3	1384.94	126.0	52.2	1544.86	226.0	107.8	1535.29
28.0	-2.2	1390.90	128.0	53.3	1545.91	228.0	108.9	1534.03
30.0	-1.1	1396.72	130.0	54.4	1546.91	230.0	110.0	1532.74
32.0	0.0	1402.39	132.0	55.6	1547.84	232.0	111.1	1531.42
34.0	1.1	1407.91	134.0	56.7	1548.72	234.0	112.2	1530.06
36.0	2.2	1413.30	136.0	57.8	1549.53	236.0	113.3	1528.67
38.0	3.3	1418.55	138.0	58.9	1550.29	238.0	114.4	1527.26
40.0	4.4	1423.66	140.0	60.0	1550.99	240.0	115.6	1525.81
42.0	5.6	1428.64	142.0	61.1	1551.63	242.0	116.7	1524.33
44.0	6.7	1433.48	144.0	62.2	1552.21	244.0	117.8	1522.83
46.0	7.8	1438.20	146.0	63.3	1552.74	246.0	118.9	1521.29
48.0	8.9	1442.80	148.0	64.4	1553.22	248.0	120.0	1519.73
50.0	10.0	1447.27	150.0	65.6	1553.64	250.0	121.1	1518.14
52.0	11.1	1451.62	152.0	66.7	1554.01	260.0	126.7	1507.00
54.0	12.2	1455.85	154.0	67.8	1554.32	270.0	132.2	1497.00
56.0	13.3	1459.97	156.0	68.9	1554.59	280.0	137.8	1487.00
58.0	14.4	1463.97	158.0	70.0	1554.80	290.0	143.3	1476.00
60.0	.15.56	1467.86	160.0	71.1	1554.98	300.0	148.9	1465.00
62.0	16.7	1471.64	162.0	72.2	1555.07	310.0	154.4	1453.00
64.0	17.9	1475.31	164.0	73.3	1555.13	320.0	160.0	1440.00
66.0	18.9	1478.88	166.0	74.4	1555.15	330.0	165.6	1426.00
68.0	20.0	1482.34	168.0	75.6	1555.11	340.0	171.1	1412.00
70.0	21.1	1485.70	170.0	76.7	1555.03	350.0	176.7	1398.00
72.0	22.2	1488.96	172.0	77.8	1554.90	360.0	182.2	1383.00
74.0	23.3	1492.13	174.0	78.9	1554.72	370.0	187.8	1368.00
76.0	24.4	1495.19	176.0	80.0	1554.49	380.0	193.3	1353.00
78.0	25.6	1498.16	178.0	81.1	1554.22	390.0	198.9	1337.00
80.0	26.7	1501.04	180.0	82.2	1553.91	400.0	204.4	1320.00
82.0	27.8	1503.82	182.0	83.3	1553.55	410.0	210.0	1302.00
84.0	28.9	1506.52	184.0	84.4	1553.14	420.0	215.6	1283.00
86.0	30.0	1509.13	186.0	85.6	1552.70	430.0	221.1	1264.00
88.0	31.1	1511.65	188.0	86.7	1552.21	440.0	226.7	1244.00
90.0	32.2	1514.08	190.0	87.8	1551.67	450.0	232.2	1220.00
90.0		1516.44	192.0	88.9	1551.10	460.0	237.8	1220.00
	33.3 34.4	1518.70	192.0	90.0	1550.48	470.0	243.3	1180.00
94.0		1520.89	194.0	90.0	1549.82	480.0	243.3	1160.00
96.0 98.0	35.6 36.7	1523.00	198.0	92.2	1549.02	490.0	240.9	1140.00